

(12) **United States Patent**  
**Gabbay**

(10) **Patent No.:** **US 6,264,691 B1**  
(45) **Date of Patent:** **Jul. 24, 2001**

(54) **APPARATUS AND METHOD FOR SUPPORTING A HEART VALVE**

(76) Inventor: **Shlomo Gabbay**, #1 Randall Dr., Short Hills, NJ (US) 07078

(\*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 0 days.

(21) Appl. No.: **09/298,493**

(22) Filed: **Apr. 23, 1999**

(51) **Int. Cl.<sup>7</sup>** ..... **A61F 2/24**

(52) **U.S. Cl.** ..... **623/2.14; 623/2.18; 623/2.38; 623/904; 600/37**

(58) **Field of Search** ..... **623/2.38, 2.39, 623/2.4, 2.12-2.19, 900, 904; 600/37**

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

3,570,014	3/1971	Hancock .	
3,739,402	6/1973	Cooley et al. .	
4,035,849	7/1977	Angell et al. .	
4,477,930	10/1984	Totten et al. .	
4,759,758	7/1988	Gabbay .	
5,032,128	7/1991	Alonso .	
5,156,621	10/1992	Navia et al. .	
5,545,215 *	8/1996	Duran .....	623/2.1 X
5,584,879	12/1996	Reimold et al. .	

**FOREIGN PATENT DOCUMENTS**

95/28899 \* 11/1995 (WO) ..... 623/2.19

**OTHER PUBLICATIONS**

“An Appraisal of the Ross Procedure: Goals & Technical Guidelines”, *Operative Techniques in Cardiac & Thoracic Surgery*, vol. 2, No. 4, Nov. 1997; pp. 289-301.

“Modified Pulmonary Autograft Aortic Root Replacement: The Sinus Obliteration Technique”, Michael D. Black, MD, Jacques A. M. von Son, MD, PhD & Frank L. Hanley, MD, *The Society of Thoracic Surgeons*, 1995; 60:1434-6.

\* cited by examiner



*Primary Examiner*—David H. Willse

(74) *Attorney, Agent, or Firm*—Amin & Turocy, LLP

(57) **ABSTRACT**

An apparatus and method are disclosed for supporting a heart valve with a flexible girdle. The girdle has an elongated cylindrical sidewall having an axial length at least commensurate with the heart valve. The girdle is disposed around a tubular valve wall of the heart valve being implanted so that the inflow end of the girdle is adjacent the inflow end of the tubular valve wall. The inflow ends of the girdle and heart valve may then be sutured together to implant the valve. The girdle provides support to stabilize the heart valve and inhibit deformation thereof.

**44 Claims, 3 Drawing Sheets**

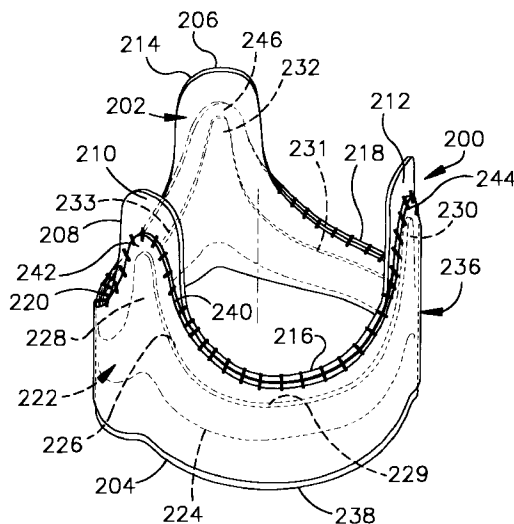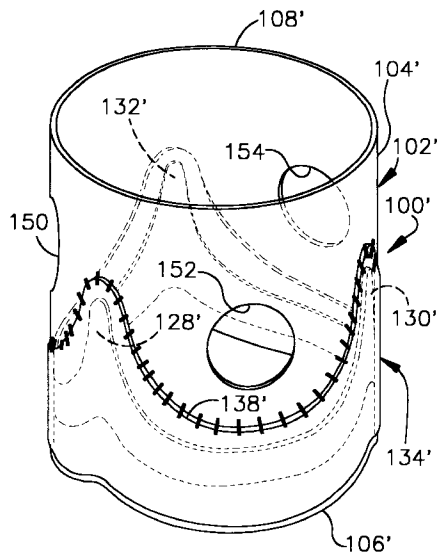

**NORRED EXHIBIT 2209 - Page 1**  
**Medtronic, Inc., Medtronic Vascular, Inc.,**  
**& Medtronic Corevalve, LLC**  
**v. Troy R. Norred, M.D.**  
**Case IPR2014-00111**

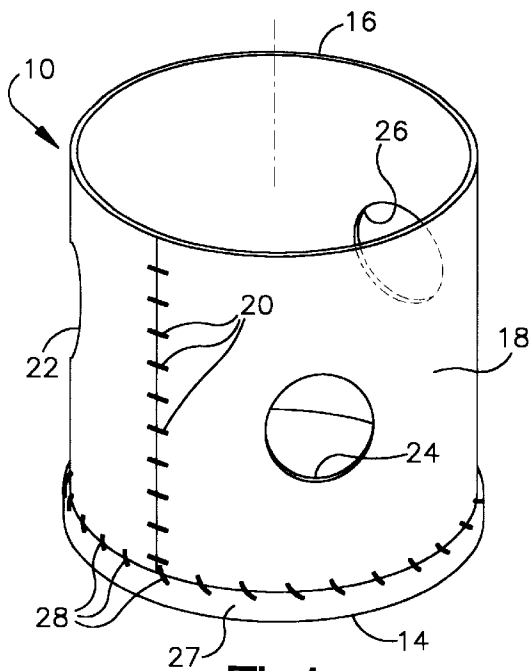


Fig.1

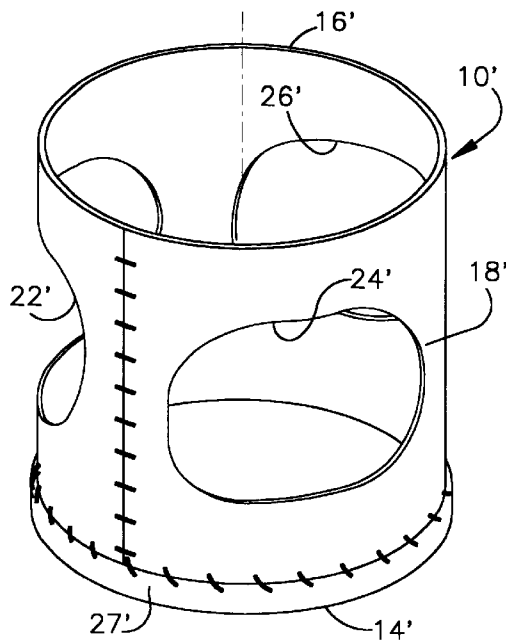


Fig.2

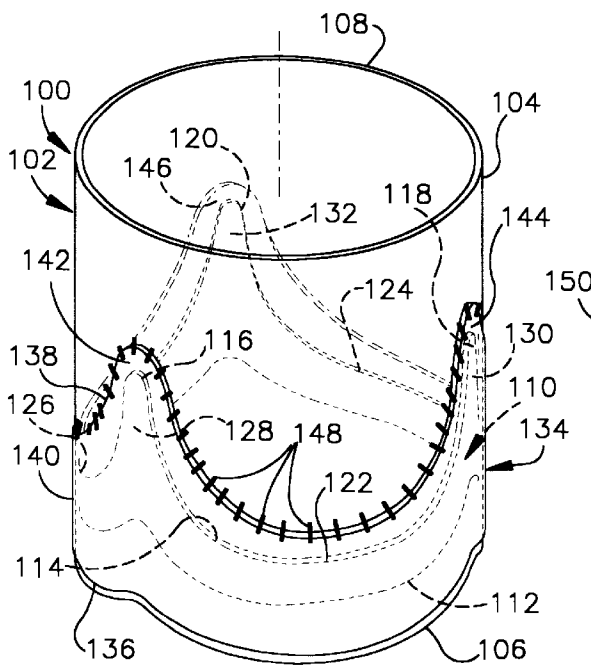


Fig.3

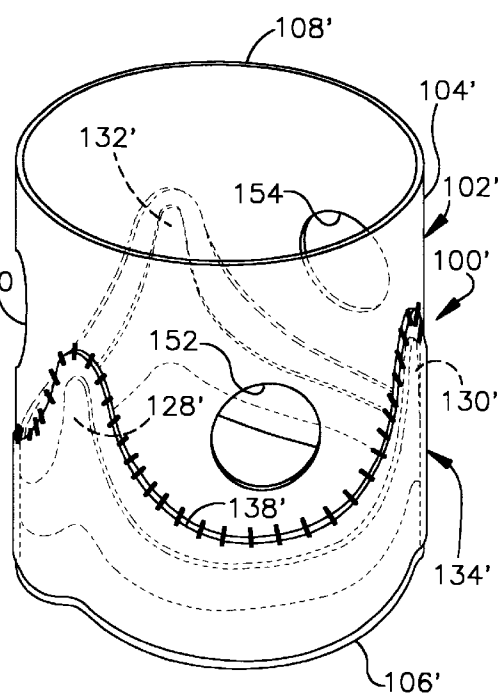


Fig.4

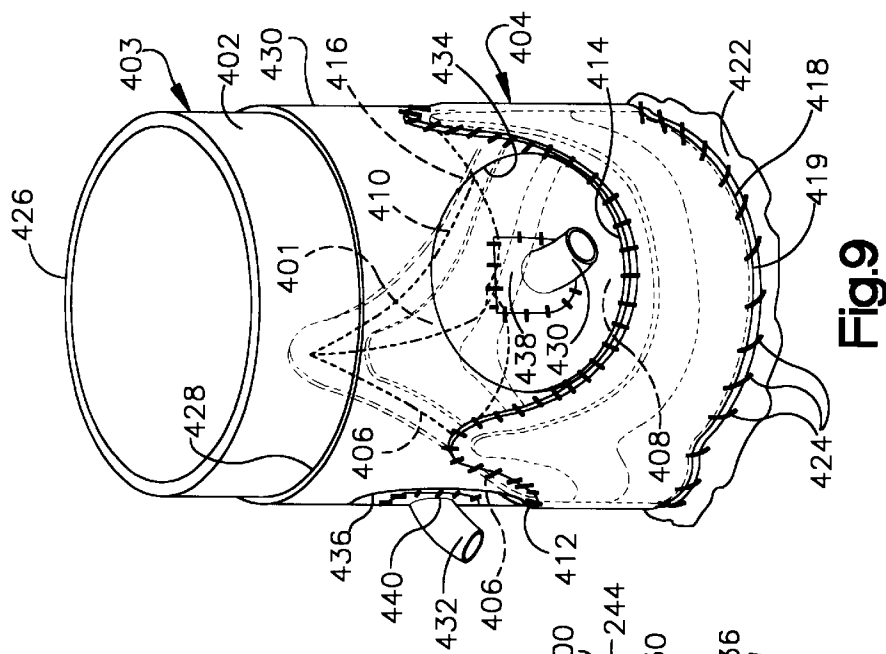


Fig.5

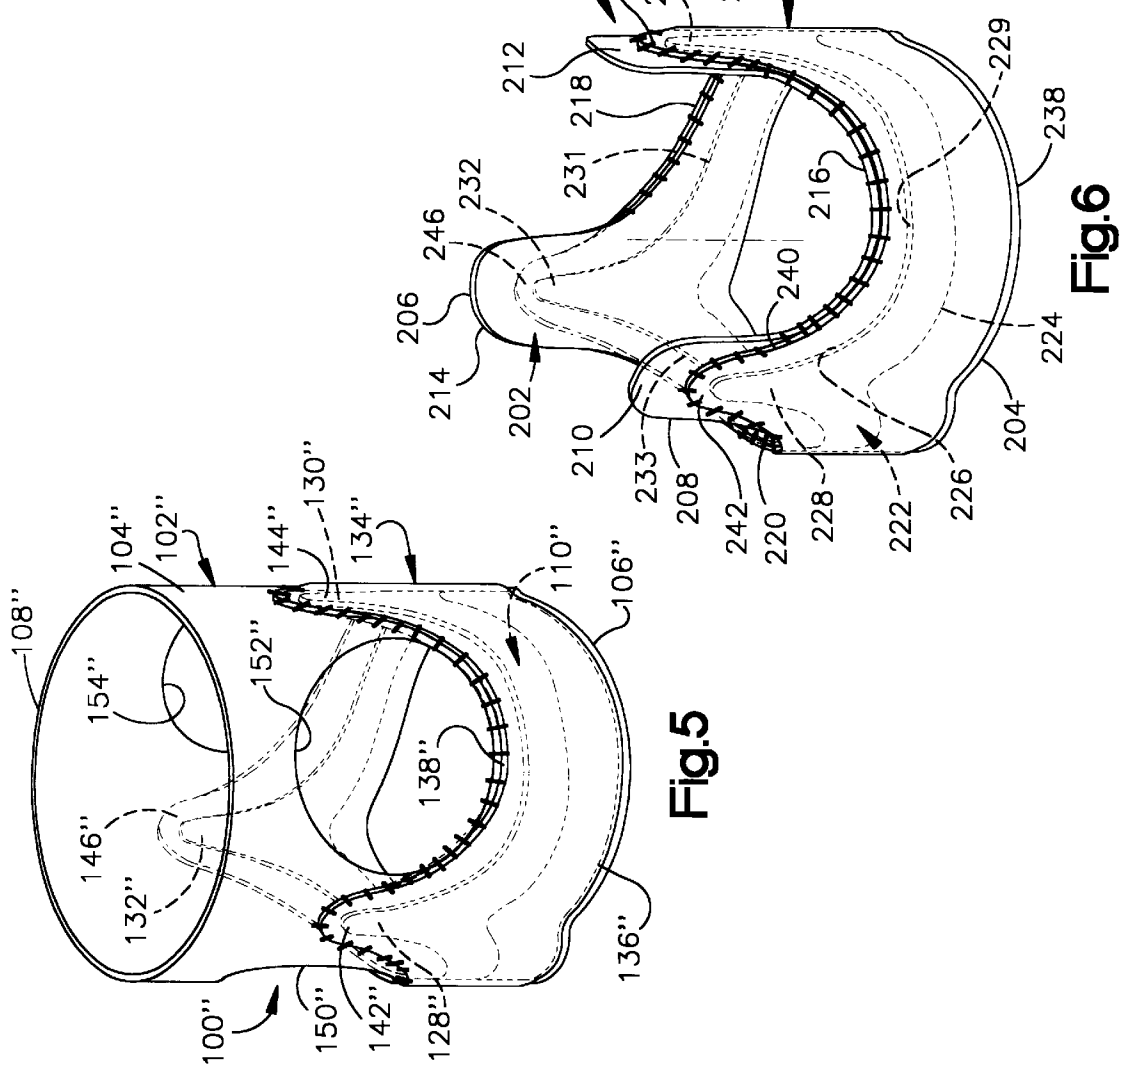


Fig.6



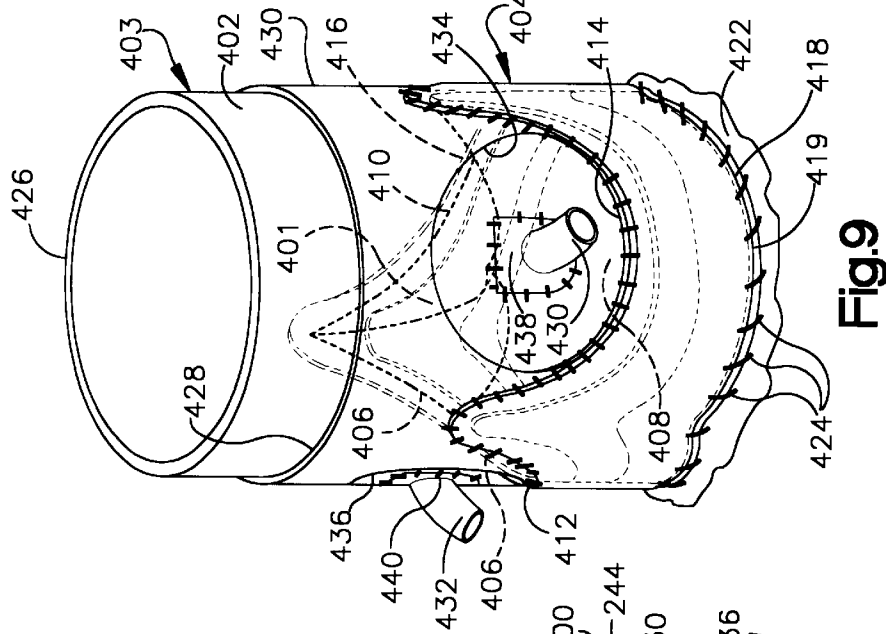


Fig.9

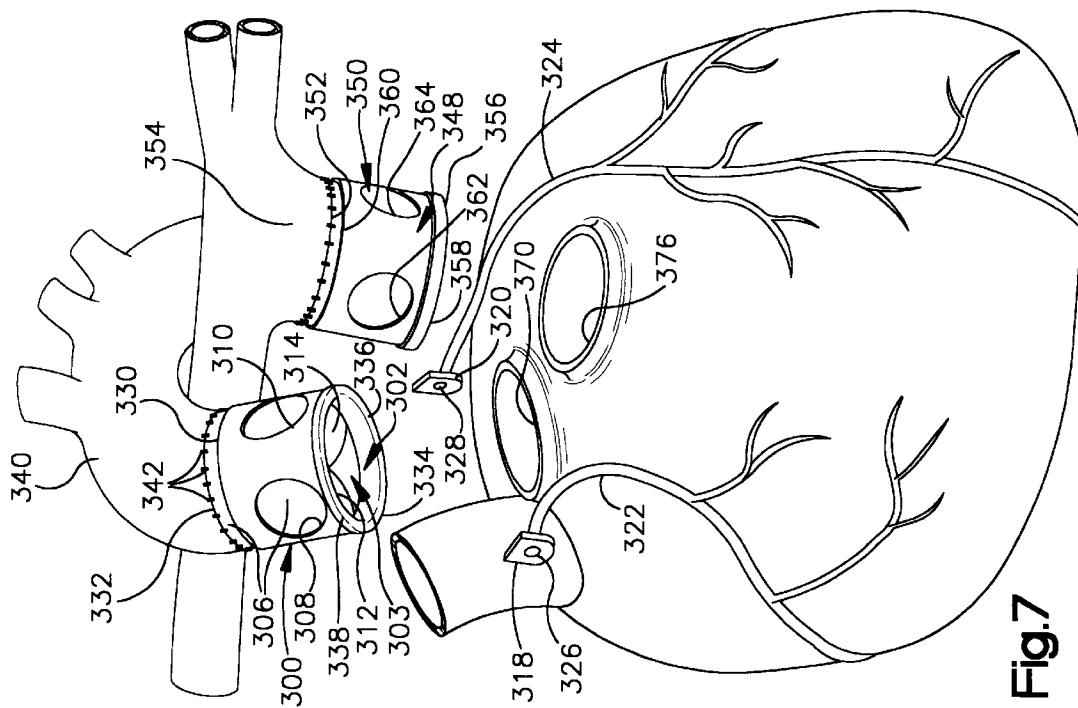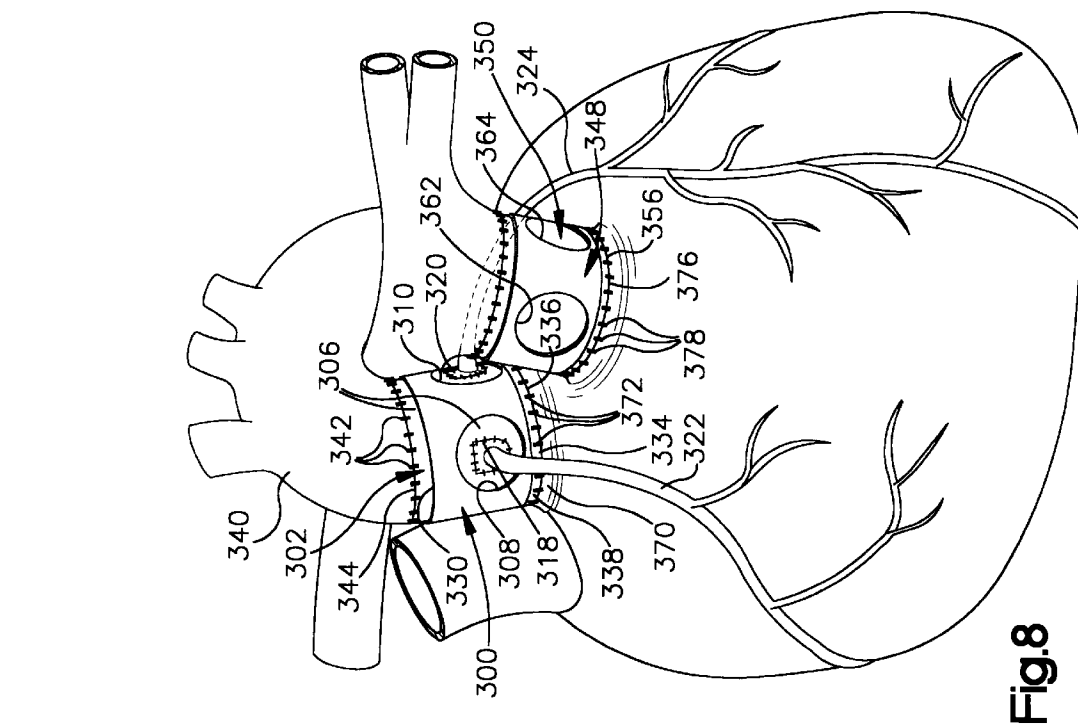

1

## APPARATUS AND METHOD FOR SUPPORTING A HEART VALVE

### CROSS REFERENCE TO RELATED APPLICATION

This application is related to U.S. patent application Ser. No. 09/1052,707, now U.S. Pat. No. 5,935,163, which was filed Mar. 31, 1998 and entitled Natural Tissue Heart Valve Prosthesis.

### TECHNICAL FIELD

The present invention relates to an apparatus and method for supporting a heart valve. More particularly, the present invention relates to an apparatus and method for supporting a heart valve by disposing a girdle externally about the valve.

### BACKGROUND OF THE INVENTION

The use of a patient's healthy pulmonic valve as an autograft to replace a diseased aortic valve has been gaining worldwide acceptance as a viable alternative for replacing the patient's diseased aortic valve. This procedure is known as the Ross procedure after the surgeon who introduced the procedure in 1967.

The Ross procedure is performed by transplanting a patient's healthy pulmonic valve along with a portion of the pulmonary artery to replace the aortic valve and a few centimeters of the aorta. The left and right coronary arteries are attached to the valve wall of the pulmonary autograft after making small slits through the valve wall into coronary sinuses of the autograft.

The pulmonic valve is typically replaced by a homograft, such as a pulmonic or aortic heart valve from a cadaver. The Ross procedure is preferred over other heart valve replacement procedures, especially for individuals who are unable to take anticoagulation drugs. The Ross procedure has received substantial discussion in various publications.

For example, Oury et al., An Appraisal of the Ross Procedure: Goals and Technical Guidelines, Operative Techniques in Cardiac and Thoracic Surgery, Vol. 2, No. 4 (November), 1997: pp. 289-301, describes the Ross procedure as well as some alternative techniques for performing the procedure.

Black et al., Modified Pulmonary Autograft Aortic Root Replacement: The Sinus Obliteration Technique, Ann Thoracic Surgery, 1995; 60:1434-1436, describes a rather complicated technique to remedy a frequent problem of dilation of the pulmonary autograft following the Ross procedure. This approach utilizes large coronary buttons to replace the pulmonary sinus completely and leaves the non-coronary aortic sinus to support the non-coronary sinus of the pulmonary autograft.

### SUMMARY OF THE INVENTION

The present invention is directed to an external support apparatus for a heart valve that is disposed within an elongated tubular valve wall. The apparatus includes a girdle having an elongated cylindrical sidewall with inflow and outflow ends that are spaced apart an axial length that is at least substantially commensurate with the axial length of the heart valve disposed within the tubular valve wall.

Preferably, at least two apertures are formed through the sidewall of the girdle and spaced axially from the inflow end thereof. The apertures are spaced circumferentially apart for

2

generally radial alignment with corresponding sinuses of the heart valve which is to be supported by the girdle. The inflow end of the girdle preferably is folded toward the outflow end to provide additional support at its inflow end.

In another embodiment, the girdle, as described above, is further supported by a stent disposed externally about the sidewall of the girdle.

Yet another embodiment of the present invention is directed to a method for improving implantation of a heart valve having inflow and outflow ends and located within a tubular valve wall. An elongated cylindrical girdle is disposed about the tubular valve wall and the heart valve located therein so as to inhibit deformation of the heart valve. The girdle has a cylindrical sidewall portion with inflow and outflow ends spaced apart an axial length at least substantially commensurate with the axial length of the heart valve located within the tubular valve wall. The inflow end of the girdle is positioned adjacent the inflow end of the tubular valve wall. During implantation of the heart valve, the inflow ends of the valve and girdle preferably are secured together to an outflow annulus of the heart.

### BRIEF DESCRIPTION OF THE DRAWINGS

The foregoing and other features and advantages of the present invention will become apparent to those skilled in the art to which the present invention relates upon reading the following description with reference to the accompanying drawings, wherein:

FIG. 1 is a first embodiment of an apparatus in accordance with the present invention;

FIG. 2 is a second embodiment of an apparatus in accordance with the present invention;

FIG. 3 is a third embodiment of an apparatus in accordance with the present invention;

FIG. 4 is a fourth embodiment of an apparatus in accordance with the present invention;

FIG. 5 is a fifth embodiment of an apparatus in accordance with the present invention;

FIG. 6 is a sixth embodiment of an apparatus in accordance with the present invention;

FIG. 7 is an isometric view of the apparatus of FIG. 1 mounted to a heart valve being implanted to a patient's heart;

FIG. 8 is an isometric view, similar to FIG. 7, illustrating a completed heart valve transplant procedure using the apparatus of FIG. 1; and

FIG. 9 is an isometric view of the apparatus of FIG. 5 disposed about a heart valve in accordance with the present invention.

### DESCRIPTION OF PREFERRED EMBODIMENTS

FIG. 1 illustrates a first embodiment of a heart valve girdle **10** in accordance with the present invention. The girdle **10** has an inflow end **14** and an outflow end **16** spaced apart by a length of a cylindrical sidewall **18**. The terms "inflow" and "outflow" are used herein to refer to ends of the girdle which are to be positioned at corresponding ends of a heart valve.

Because the girdle **10** is to be mounted externally about a heart valve, such as an autogenous or homogenous heart valve disposed within a length of a tubular valve wall, the axial length of the sidewall **18** is at least substantially commensurate with the axial length of the heart valve which

# Explore Litigation Insights

Docket Alarm provides insights to develop a more informed litigation strategy and the peace of mind of knowing you're on top of things.

## Real-Time Litigation Alerts



Keep your litigation team up-to-date with **real-time alerts** and advanced team management tools built for the enterprise, all while greatly reducing PACER spend.

Our comprehensive service means we can handle Federal, State, and Administrative courts across the country.

## Advanced Docket Research



With over 230 million records, Docket Alarm's cloud-native docket research platform finds what other services can't. Coverage includes Federal, State, plus PTAB, TTAB, ITC and NLRB decisions, all in one place.

Identify arguments that have been successful in the past with full text, pinpoint searching. Link to case law cited within any court document via Fastcase.

## Analytics At Your Fingertips



Learn what happened the last time a particular judge, opposing counsel or company faced cases similar to yours.

Advanced out-of-the-box PTAB and TTAB analytics are always at your fingertips.

## API

Docket Alarm offers a powerful API (application programming interface) to developers that want to integrate case filings into their apps.

## LAW FIRMS

Build custom dashboards for your attorneys and clients with live data direct from the court.

Automate many repetitive legal tasks like conflict checks, document management, and marketing.

## FINANCIAL INSTITUTIONS

Litigation and bankruptcy checks for companies and debtors.

## E-DISCOVERY AND LEGAL VENDORS

Sync your system to PACER to automate legal marketing.