


## **Edwards SAPIEN 3 Transcatheter Heart Valve with the Edwards Commander Delivery System**

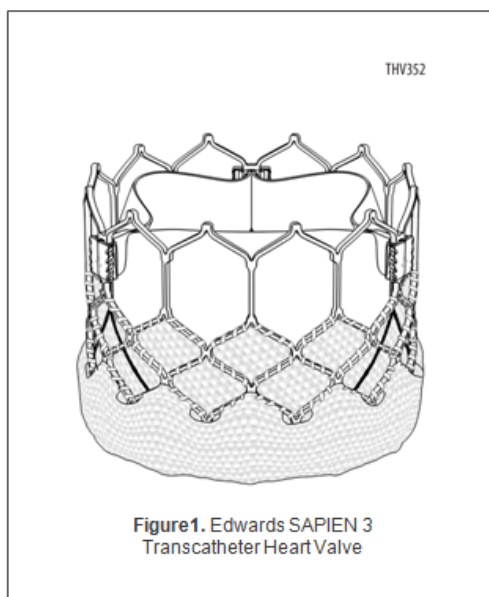

### **Instructions for Use**

**CAUTION:** Federal (USA) law restricts these devices to sale by or on the order of a physician.

Implantation of the transcatheter heart valve should be performed only by physicians who have received Edwards Lifesciences training. The implanting physician should be experienced in balloon aortic valvuloplasty.

Please verify that you have the latest version of the instructions for use prior to using the device by visiting <http://THVIFU.edwards.com> or by calling 1.800.822.9837. In order to access the instructions for use, an IFU Code will be required.

**STERILE:** The THV is supplied sterilized with glutaraldehyde solution. The delivery system, eSheath introducer set, and crimper are supplied sterilized with ethylene oxide gas.

**Edwards Lifesciences v. Boston Scientific  
U.S. Patent No. 6,915,560  
IPR2017-00444 EX. 2032**

Edwards, Edwards Lifesciences, the stylized E logo, Carpentier-Edwards, Edwards Commander, Edwards eSheath, Edwards SAPIEN, Edwards SAPIEN 3, eSheath, Qualcrimp, PARTNER, PARTNER II, SAPIEN, SAPIEN 3, TFX and ThermoFix are trademarks of Edwards Lifesciences Corporation.

## 1.0 Device Description

### • Edwards SAPIEN 3 Transcatheter Heart Valve- Model 9600TFX (Figure 1)

The Edwards SAPIEN 3 Transcatheter Heart Valve (THV) is comprised of a balloon-expandable, radiopaque, cobalt-chromium frame, trileaflet bovine pericardial tissue valve, and polyethylene terephthalate (PET) fabric skirt. The leaflets are treated according to the Carpentier-Edwards ThermaFix process.

Table 1

Valve Size	Height
20 mm	15.5 mm
23 mm	18 mm
26 mm	20 mm
29 mm	22.5 mm

Table 2

Native Valve Annulus Size (TEE)	Native Valve Annulus Size (CT)		THV Size
	Area	Area Derived Diameter	
16-19 mm	273 – 345 mm <sup>2</sup>	18.6-21 mm	20 mm
18-22 mm	338 – 430 mm <sup>2</sup>	20.7-23.4 mm	23 mm
21-25 mm	430 – 546 mm <sup>2</sup>	23.4-26.4 mm	26 mm
24-28 mm	540 – 683 mm <sup>2</sup>	26.2-29.5 mm	29 mm
THV size recommendations are based on native valve annulus size, as measured by transesophageal echocardiography (TEE) or computed tomography (CT). Patient anatomical factors and multiple imaging modalities should be considered during THV size selection. Note: Risks associated with undersizing and oversizing should be considered.			


### • Edwards Commander Delivery System (Figure 2)

The Edwards Commander delivery system (usable length 105 cm) is used for delivery of the Edwards SAPIEN 3 transcatheter heart valve and consists of a Flex Catheter to aid in valve alignment to the balloon, tracking, and positioning of the THV. The delivery system includes a tapered tip to facilitate crossing of the native valve. The handle contains a Flex Wheel to control flexing of the Flex Catheter, and a Balloon Lock and Fine Adjustment Wheel to facilitate valve alignment and positioning of the valve within the native annulus. A stylet is included within the guidewire lumen of the delivery system. The Balloon Catheter has radiopaque Valve Alignment Markers defining the working length of the balloon. A radiopaque Center Marker in the balloon is provided to help with valve positioning. A radiopaque Triple Marker proximal to the balloon indicates the Flex Catheter position during deployment. The inflation parameters for THV deployment are:

Table 3

Model	Nominal Balloon Diameter	Nominal Inflation Volume	Rated Burst Pressure (RBP)
9600LDS20	20 mm	11 mL	7 atm
9600LDS23	23 mm	17 mL	7 atm
9600LDS26	26 mm	23 mL	7 atm
9600LDS29	29 mm	33 mL	7 atm


Figure 2 Edwards Commander Delivery System

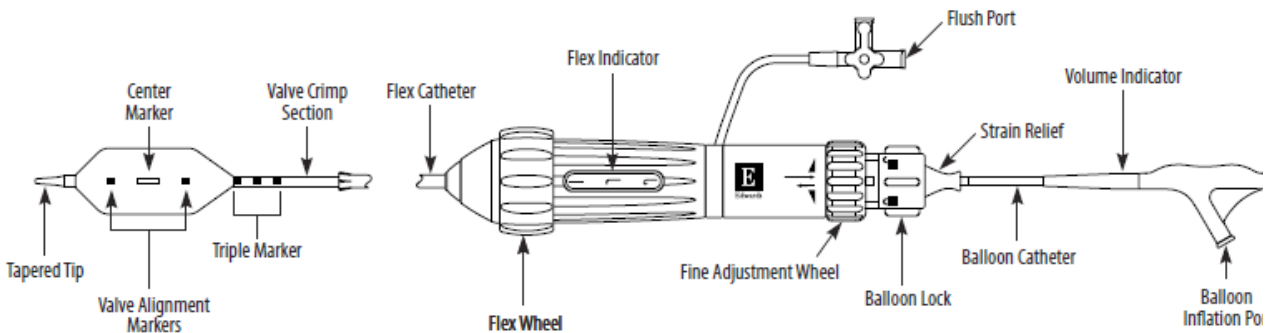

- **Qualcrimp Crimping Accessory (Figure 3)**

The Qualcrimp crimping accessory (packaged with the Edwards Commander delivery system) is used during crimping of the THV.

Figure 3

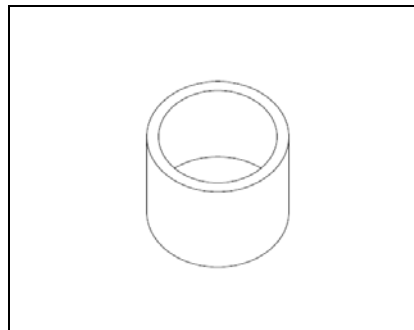

Laminated Qualcrimp

- **Edwards eSheath Introducer Set**

Refer to the Edwards eSheath Introducer Set for device description.

- **Edwards Crimper**

Refer to the Edwards Crimper instructions for use for device description.

## 2.0 Indications

The Edwards SAPIEN 3 Transcatheter Heart Valve (THV), model 9600TFX, and accessories are indicated for relief of aortic stenosis in patients with symptomatic heart disease due to severe native calcific aortic stenosis who are judged by a heart team, including a cardiac surgeon, to be at high or greater risk for open surgical therapy (i.e., Society of Thoracic Surgeons operative risk score  $\geq 8\%$  or at a  $\geq 15\%$  risk of mortality at 30 days).

### 3.0 Contraindications

The THV and delivery systems are contraindicated in patients who cannot tolerate an anticoagulation/antiplatelet regimen or who have active bacterial endocarditis or other active infections.

### 4.0 Warnings

- Observation of the pacing lead throughout the procedure is essential to avoid the potential risk of pacing lead perforation.
- There is an increased risk of stroke in transcatheter aortic valve replacement procedures, as compared to balloon aortic valvuloplasty or other standard treatments.
- The devices are designed, intended, and distributed for single use only. **Do not resterilize or reuse the devices.** There are no data to support the sterility, nonpyrogenicity, and functionality of the devices after reprocessing.
- Incorrect sizing of the THV may lead to paravalvular leak, migration, embolization and/or annular rupture.
- Accelerated deterioration of the THV may occur in patients with an altered calcium metabolism.
- Prior to delivery, the THV must remain hydrated at all times and cannot be exposed to solutions other than its shipping storage solution and sterile physiologic rinsing solution. THV leaflets mishandled or damaged during any part of the procedure will require replacement of the THV.
- Caution should be exercised in implanting a THV in patients with clinically significant coronary artery disease.
- Patients with pre-existing mitral valve devices should be carefully assessed prior to implantation of the THV to ensure proper THV positioning and deployment.
- Do not use the THV if the tamper evident seal is broken, the storage solution does not completely cover the THV, the temperature indicator has been activated, the THV is damaged, or the expiration date has elapsed.
- Do not mishandle the delivery system or use it if the packaging or any components are not sterile, have been opened or are damaged (e.g. kinked or stretched), or the expiration date has elapsed.
- Use of excessive contrast media may lead to renal failure. Measure the patient's creatinine level prior to the procedure. Contrast media usage should be monitored.
- Patient injury could occur if the delivery system is not un-flexed prior to removal.
- Care should be exercised in patients with hypersensitivities to cobalt, nickel, chromium, molybdenum, titanium, manganese, silicon, and/or polymeric materials.
- The procedure should be conducted under fluoroscopic guidance. Some fluoroscopically guided procedures are associated with a risk of radiation injury to the skin. These injuries may be painful, disfiguring, and long-lasting.
- THV recipients should be maintained on anticoagulant/antiplatelet therapy, except when contraindicated, as determined by their physician. This device has not been tested for use without anticoagulation.
- Do not add or apply antibiotics to the storage solution, rinse solutions, or to the THV.

### 5.0 Precautions

- Long-term durability has not been established for the THV. Regular medical follow-up is advised to evaluate THV performance.
- Glutaraldehyde may cause irritation of the skin, eyes, nose and throat. Avoid prolonged or repeated exposure to, or breathing of, the solution. Use only with adequate ventilation. If skin contact occurs, immediately flush the affected area with water; in the event of contact with eyes, seek immediate medical attention. For more information about glutaraldehyde exposure, refer to the Material Safety Data Sheet available from Edwards Lifesciences.

- To maintain proper valve leaflet coaptation, do not overinflate the deployment balloon.
- Appropriate antibiotic prophylaxis is recommended post-procedure in patients at risk for prosthetic valve infection and endocarditis.
- Safety, effectiveness, and durability have not been established for valve-in-valve procedures.
- Safety and effectiveness have not been established for patients with the following characteristics/comorbidities:
  - Non-calcified aortic annulus
  - Severe ventricular dysfunction with ejection fraction < 20%
  - Congenital unicuspid or congenital bicuspid aortic valve
  - Mixed aortic valve disease (aortic stenosis and aortic regurgitation with predominant aortic regurgitation > 3+)
  - Pre-existing prosthetic heart valve or prosthetic ring in any position
  - Severe mitral annular calcification (MAC), severe (> 3+) mitral insufficiency, or Gorlin syndrome
  - Blood dyscrasias defined as: leukopenia (WBC < 3000 cells/mL), acute anemia (Hb < 9 g/dL), thrombocytopenia (platelet count < 50,000 cells/mL), or history of bleeding diathesis or coagulopathy
  - Hypertrophic cardiomyopathy with or without obstruction (HOCM)
  - Echocardiographic evidence of intracardiac mass, thrombus, or vegetation
  - A known hypersensitivity or contraindication to aspirin, heparin, ticlopidine (Ticlid™), or clopidogrel (Plavix™), or sensitivity to contrast media, which cannot be adequately premedicated
  - Significant aortic disease, including abdominal aortic or thoracic aneurysm defined as maximal luminal diameter 5 cm or greater; marked tortuosity (hyperacute bend), aortic arch atheroma (especially if thick [> 5 mm], protruding, or ulcerated) or narrowing (especially with calcification and surface irregularities) of the abdominal or thoracic aorta, severe “unfolding” and tortuosity of the thoracic aorta
  - Access characteristics that would preclude safe placement of 14F or 16F Edwards eSheath Introducer Set, such as severe obstructive calcification, severe tortuosity or diameter less than 5.5 mm or 6 mm, respectively
  - Bulky calcified aortic valve leaflets in close proximity to coronary ostia

## 6.0 Potential Adverse Events

Potential risks associated with the overall procedure including potential access complications associated with standard cardiac catheterization, balloon valvuloplasty, the potential risks of conscious sedation and/or general anesthesia, and the use of angiography:

- Death
- Stroke/transient ischemic attack, clusters or neurological deficit
- Paralysis
- Permanent disability
- Respiratory insufficiency or respiratory failure
- Hemorrhage requiring transfusion or intervention
- Cardiovascular injury including perforation or dissection of vessels, ventricle, myocardium or valvular structures that may require intervention
- Pericardial effusion or cardiac tamponade



# Explore Litigation Insights

Docket Alarm provides insights to develop a more informed litigation strategy and the peace of mind of knowing you're on top of things.

## Real-Time Litigation Alerts



Keep your litigation team up-to-date with **real-time alerts** and advanced team management tools built for the enterprise, all while greatly reducing PACER spend.

Our comprehensive service means we can handle Federal, State, and Administrative courts across the country.

## Advanced Docket Research



With over 230 million records, Docket Alarm's cloud-native docket research platform finds what other services can't. Coverage includes Federal, State, plus PTAB, TTAB, ITC and NLRB decisions, all in one place.

Identify arguments that have been successful in the past with full text, pinpoint searching. Link to case law cited within any court document via Fastcase.

## Analytics At Your Fingertips



Learn what happened the last time a particular judge, opposing counsel or company faced cases similar to yours.

Advanced out-of-the-box PTAB and TTAB analytics are always at your fingertips.

## API

Docket Alarm offers a powerful API (application programming interface) to developers that want to integrate case filings into their apps.

## LAW FIRMS

Build custom dashboards for your attorneys and clients with live data direct from the court.

Automate many repetitive legal tasks like conflict checks, document management, and marketing.

## FINANCIAL INSTITUTIONS

Litigation and bankruptcy checks for companies and debtors.

## E-DISCOVERY AND LEGAL VENDORS

Sync your system to PACER to automate legal marketing.