

US005564417A

United States Patent [19]

Chance

[11] Patent Number:

5,564,417

[45] Date of Patent:

* Oct. 15, 1996

[54] PATHLENGTH CORRECTED OXIMETER AND THE LIKE

[75] Inventor: Britton Chance, Marathon, Fla.

[73] Assignee: Non-Invasive Technology, Inc.,

Philadelphia, Pa.

[*] Notice: The term of this patent shall not extend

beyond the expiration date of Pat. No.

5,553,614.

[21] Appl. No.: 31,945

[22] Filed: Mar. 16, 1993

Related U.S. Application Data

[63] Continuation-in-part of Ser. No. 645,590, Jan. 24, 1991.

[51] Int. Cl.⁶ A61N 5/02

[52] **U.S. Cl.** **128/633**; 128/637; 128/664; 128/665; 356/39; 356/341; 356/432

5, 51, 39, 72, 319, 320, 323, 341, 432–436,

[56] References Cited

U.S. PATENT DOCUMENTS

3,638,640	2/1972	Shaw	128/633
4,223,680	9/1980	Jobsis .	
4,281,645	8/1981	Jobsis .	
4,321,930	3/1982	Jobsis et al	
4,380,240	4/1983	Jobsis et al	
4,510,938	4/1985	Jobsis et al	
4,714,341	12/1987	Hamaguri et al	
4,800,495	1/1989	Smith .	
4,800,885	1/1989	Johnson .	
4,805,623	2/1989	Jobsis .	
4,824,242	4/1989	Frick et al	
4,827,934	5/1989	Parker	128/633
4,972,331	11/1990	Chance .	
5,119,815	6/1992	Chance .	
5,167,230	12/1992	Chance .	
5,187,672	2/1993	Chance et al	

FOREIGN PATENT DOCUMENTS

WO92/20273 11/1992 WIPO .

OTHER PUBLICATIONS

Chance et al., "Photon Migration in Muscle and Brain", *Photon Migration in Tissues*, Academic Press/ New York 1989.

Chance, "Rapid and Sensitive Apectrophotometry, I. The Accelerated and Stopped–Flow Methods for the Measurement of the Reaction Kinetics, etc.", *The Review of Scientific Instruments*, 22:619–638 (1951).

Cui et al., "Experimental Study of Migration Depth for the Photons Measured at Sample Surface", *Proceedings of Time-Resolved Spectroscopy and Imaging of Tissues*, SPIE, 1413: 180–191 (1991).

Lakowicz, "Gigahertz Frequency-Domain Fluorometry: Resolution of Complex Intensity Decays, Picosecond Processes and Future Developments", *Photon Migration in Tissues*, pp. 169–185.


(List continued on next page.)

Primary Examiner—David M. Shay Attorney, Agent, or Firm—Fish & Richardson P.C.

57] ABSTRACT

A pathlength corrected spectrophotometer for tissue examination includes an oscillator for generating a carrier waveform of a selected frequency, an LED light source for generating light of a selected wavelength that is intensity modulated at the selected frequency introduced to a subject, and a photodiode detector for detecting light that has migrated in the tissue of the subject. The spectrophotometer also includes a phase detector for measuring a phase shift between the introduced and detected light, a magnitude detector for determination of light attenuation in the examined tissue, and a processor adapted to calculate the photon migration pathlength and determine a physiological property of the examined tissue based on the pathlength and on the attenuation data.

30 Claims, 7 Drawing Sheets





OTHER PUBLICATIONS

Sevick et al., "Analysis of absorption, scattering, and hemoglobin saturation using phase modulation spectroscopy", *Proceedings of Time-Resolved Spectroscopy and Imaging Tissues*, SPIE, 1431:264–275 (1991).

Sevick et al., "Photon migration in a model of the head measured using time-and frequency-domain, etc.", *Proceedings of Time-Resolved Spectroscopy and Imaging Tissues*, SPIE, 1431:84–96 (1991).


Sevick et al., "Quantitation of Time- and Frequency-Resolved Optical Spectra for the Determination of Tissue

Oxygenation", Analytical Biochemistry, 195:001-0022 (1991).

Van der Zee et al., "Computed Point Spread Functions for Light in Tissue Using a Measured Volume Scattering Function", Advances in Experimental Medicine and Biology: Oxygen Transport to Tissue X, 222:191–197 (1988).

Weng et al., "Measurement of Biological Tissue Metabolism Using Phase Modulation Spectroscopic Technology", *Proceedings of Time-Resolved Spectroscopy and Imaging of Tissues*, SPIE, 1431: 161–170 (1991).



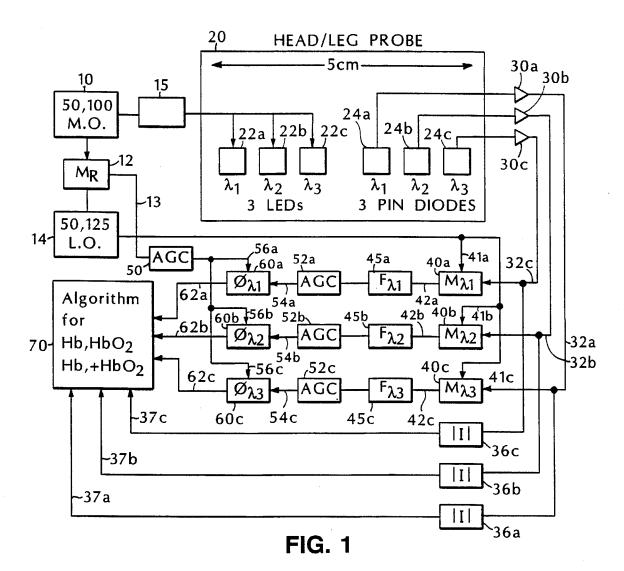




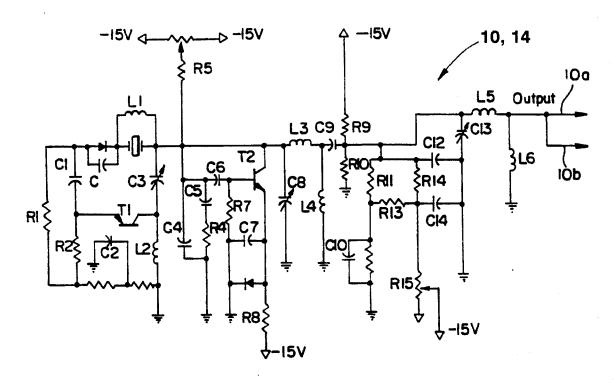


FIG. 2



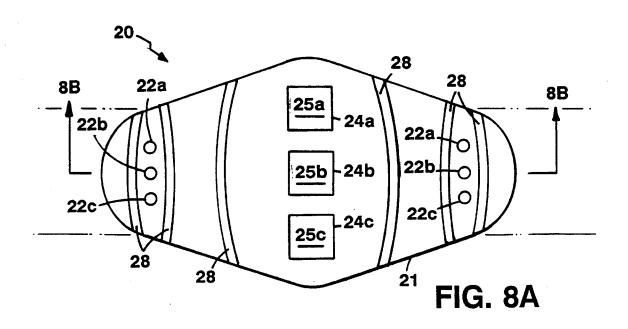

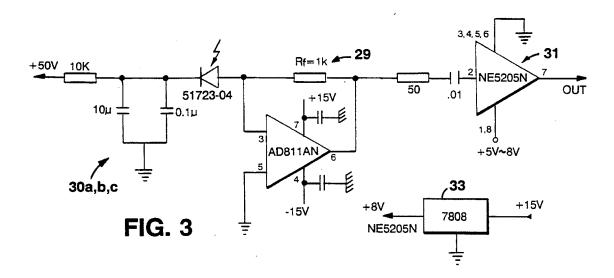

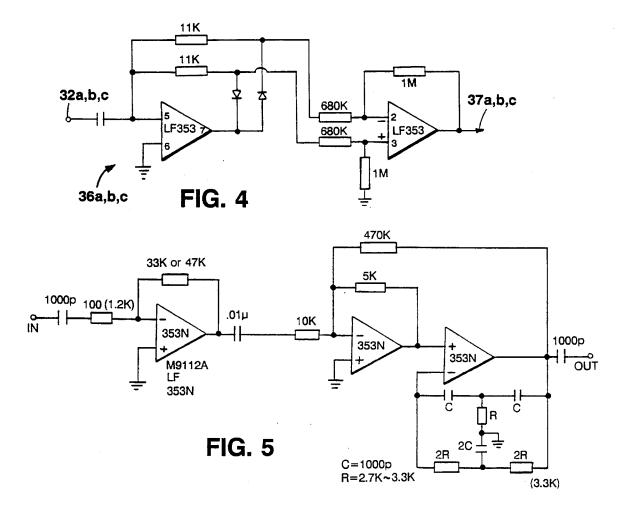

DOCKET

Explore Litigation Insights



Docket Alarm provides insights to develop a more informed litigation strategy and the peace of mind of knowing you're on top of things.

Real-Time Litigation Alerts



Keep your litigation team up-to-date with **real-time** alerts and advanced team management tools built for the enterprise, all while greatly reducing PACER spend.

Our comprehensive service means we can handle Federal, State, and Administrative courts across the country.

Advanced Docket Research



With over 230 million records, Docket Alarm's cloud-native docket research platform finds what other services can't. Coverage includes Federal, State, plus PTAB, TTAB, ITC and NLRB decisions, all in one place.

Identify arguments that have been successful in the past with full text, pinpoint searching. Link to case law cited within any court document via Fastcase.

Analytics At Your Fingertips



Learn what happened the last time a particular judge, opposing counsel or company faced cases similar to yours.

Advanced out-of-the-box PTAB and TTAB analytics are always at your fingertips.

API

Docket Alarm offers a powerful API (application programming interface) to developers that want to integrate case filings into their apps.

LAW FIRMS

Build custom dashboards for your attorneys and clients with live data direct from the court.

Automate many repetitive legal tasks like conflict checks, document management, and marketing.

FINANCIAL INSTITUTIONS

Litigation and bankruptcy checks for companies and debtors.

E-DISCOVERY AND LEGAL VENDORS

Sync your system to PACER to automate legal marketing.

