

Determination of melting point of vegetable oils and fats by differential scanning calorimetry (DSC) technique

By Renata Tieko Nassu* and Lireny Aparecida Guaraldo Gonçalves

Laboratório de Oleos e Gorduras - Faculdade de Engenharia de Alimentos (FEA) - Universidade Estadual de Campinas (UNICAMP), Caixa Postal 6091 CEP 13081-970, Campinas, SP, Brazil.

* To whom correspondence should be addressed. New address: Centro Nacional de Pesquisa da Agroindústria Tropical (CNPAT)/EMBRAPA - Rua Dra. Sara Mesquita, 2270. CEP 60511 -110, Fortaleza, CE, Brazil. e-mail: renata@cnpat.embrapa.br

RESUMEN

Determinación del punto de fusión de aceites y grasas vegetales por técnica de calorimetría diferencial de barrido (DSC).

El punto de fusión de grasas es usado para caracterizar aceites y grasas, y está relacionado con sus propiedades físicas, tales como dureza y comportamiento térmico. El presente trabajo muestra la utilización de la técnica de Calorimetría Diferencial de Barrido (DSC) en la determinación del punto de fusión de grasas. En comparación con el punto de ablandamiento (AOCS método Cc 3-25), los valores de DSC fueron más altos que los obtenidos por los métodos de AOCS. Esto ha ocurrido debido al hecho que los valores obtenidos por la técnica de DSC fueron tomados cuando la grasa había fundido completamente. DSC fue también útil para determinar puntos de fusión de aceites líquidos, tales como los de soya y algodón.

PALABRAS-CLAVE: Calorimetría Diferencial de Barrido (DSC) — Grasa vegetal — Punto de ablandamiento — Punto de fusión.

SUMMARY

Determination of melting point of vegetable oils and fats by differential scanning calorimetry (DSC) technique.

Melting point of fats is used to characterize oils and fats and is related to their physical properties, such as hardness and thermal behaviour. The present work shows the utilization of DSC technique on the determination of melting point of fats. In a comparison with softening point (AOCS method Cc 3-25), DSC values were higher than those obtained by AOCS method. It has occurred due to the fact that values obtained by DSC technique were taken when the fat had melted completely. DSC was also useful for determining melting point of liquid oils, such as soybean and cottonseed ones.

KEY-WORDS: Differential Scanning Calorimetry (DSC) — Melting point — Softening point — Vegetable fat.

1. INTRODUCTION

Melting point of fats is measured by various methods. These include Wiley melting point (AOCS

Method Cc 2-38) (AOCS, 1988), open capillary slip point, softening point (AOCS method Cc 3-25) (AOCS, 1988), ring and ball methods and automated techniques such as Mettler dropping point and Elex apparatus. Several authors compared methods usually applied with another ones, in relation to the methods themselves and temperature procedures. Kanematsu *et al.*, (1979a and 1979b), used Mettler dropping point and tested conditions for measurement, comparing values obtained by Mettler dropping point, softening point from Japanese standard, clear point and Wiley melting point with various fats. Close correlations were found between these methods. Open-tube melting point using Elex automatic apparatus was compared with the conventional method by Kanematsu *et al.*, (1981). Results showed that the values obtained did not show statistically significant differences. Deman *et al.*, (1983) compared several methods for determination of melting point using various fats and tested the reproducibility of these methods. Reproducibilities of the Mettler dropping point and softening point were considered excellent and for slip point, poor. Kawada *et al.*, (1985) proposed melting point determination by another methods, such as ring and ball methods.

Many melting point measurement methods can be grouped in different ways. As parameters for measuring it, some methods determine the point of complete melting of all crystalline material while others use a point farther removed from there and are called softening, slipping or dropping points. Subjective interpretation of the endpoint by the operator or objective indications are used. Some methods depend upon manual controls; others employ a certain degree of automation. In this group, modern instrumentation has shown the way for possible improvements. The use of automatic temperature control, linear heating rates and objective endpoint determinations promise an improvement in the precision of melting point tests (Mertens, 1973). Differential Scanning Calorimetry

(DSC) is an alternative, being one of the most used techniques for studying thermal behaviour of various foods components. Melting point obtained by DSC is generally considered as the onset temperature, the inflection point of melting curve and solid line. Deman *et al.*, (1991) consider melting point as the peak temperature calculated from a DSC melting curve. In this referred study, temperature measured at the end of melting curve obtained by DSC was considered as the real melting point, where the melting phenomenon finishes, when all crystals in solid state became liquid. Siew *et al.*, (1982) concluded that melting point is essentially determined by the hard fraction of stearins, indicated by the major peak. Chaisery & Dimick (1995), in a study of crystallization of cocoa butter, measured melting point by DSC of low and high melting fractions, considering onset melting temperature. In a study of effect of cooling and heating rates variation, Cebula & Smith (1991) measured melting point of pure triglycerides, also considering the onset temperature.

In this study, final melting temperatures obtained by DSC technique were compared with softening point (AOCS method Cc 3-25) (AOCS, 1988) values for various vegetable oils and fats.

2. EXPERIMENTAL

2.1. Material

14 different types of oils and fats were used: soybean oil, cottonseed oil, palm oil, palm olein, palm stearin, babassu oil and hydrogenated oils (soybean, two types; palm oil, cottonseed oil and babassu oil), palm kernel oil, palm kernel stearin and intersterified cottonseed oil. The samples were gently supplied by Gessy Lever Ltda. (Valinhos, SP) and Refinadora de Oleos Brasil (Sao Caetano do Sul, SP).

2.2. Fatty acid compositions of samples

Fatty acid composition was done through analysis of methyl esters by gas-liquid chromatography. The instrument used was a Perkin Elmer Sigma 3B gas-liquid chromatograph with ionization detector and the results were obtained by a Perkin Elmer integrator LCI - 100. The methyl esters were obtained according to Hartman & Lago (1973).

2.3. Melting point measurement of samples

Melting point of samples were measured by Softening point [AOCS method Cc 3-25 (1988)] and by DSC, as described. The instrument used was a

Perkin Elmer DSC7 Differential Scanning Calorimeter. Nitrogen was the carrier gas and calibration was done with indium, after checking the operation with distilled, deionized water. 10-15mg of sample were enclosed in hermetically sealed aluminum pans and run against air (empty pan) as reference. DSC melting curves were obtained according to Dodd & Tonge (1987). Samples were heated to 80°C for 5 minutes, cooled at 10°C/min to -50°C, holding at this temperature for 5 minutes to crystallize the sample. After this procedure, melting curves were recorded from initial temperature to 80°C at a heating rate of 10°C/min. The resulting DSC data was analyzed by peak program and peak temperature, onset temperature and melting temperature were recorded. Melting temperature was considered as the temperature at the end of the curve, when melting has completed.

3. RESULTS AND DISCUSSION

Fatty acid composition of the samples can be seen in table I. Values showed the great variability of the samples, which influences melting point values and the shape of DSC melting curves.

Table I
Fatty acid composition of vegetable oils

Sample	C8:0	C10:0	C12:0	C14:0	C16:0	C16:1	C18:0	C18:1	C18:2	C18:3	C20:0
SON	—	—	—	0.12	11.41	0.11	9.51	22.31 49.21(a)	2.05 4.84(b)	0.24	0.18
SOB	—	—	—	0.12	11.16	0.11	13.04	35.02 36.28(a)	0.91 2.66(b)	0.25	0.44
AGH	—	—	—	0.84	23.31	0.74	3.36	59.39	1.12 10.11(b)	0.01	0.25 0.86(c)
AGI	5.34	4.25	35.89	13.30	11.06	—	23.67	3.77	2.71	—	—
PMD	—	—	0.46	0.82	38.23	—	5.32	42.47	12.19	0.10	0.39
PME	—	—	—	0.80	49.83	—	6.59	32.62	9.28	0.50	0.37
PMO	—	—	—	0.63	35.43	—	5.08	44.53	13.35	0.59	0.37
PMH	—	—	—	0.68	40.22	—	56.30	2.07	0.19 0.52(b)	0.01	—
PKR	4.35	3.57	48.71	16.34	8.15	—	2.34	14.30	2.22	—	—
PKE	2.62	3.02	54.85	21.06	8.35	—	2.47	6.68	0.94	—	—
BBD	6.01	5.11	43.87	16.30	9.04	—	3.51	13.73	2.43	—	—
BBH	5.90	5.07	42.74	15.54	9.08	—	15.69	2.02 2.85(a)	1.12	—	—

SON-hydrogenated soybean oil type «N»; SOB-hydrogenated soybean oil type «B»; AGH-hydrogenated cottonseed oil; AGI-interesterified cottonseed oil; PMD-deodorized palm oil; PME-palm stearin; PMO-palm olein; PMH-hydrogenated palm oil; PKR-refined palm kernel oil; PKE-palm kernel stearin; BBD-deodorized babassu oil; BBH-hydrogenated babassu oil.

C8:0 - Caprylic acid
C10:0 - Capric acid
C12:0 - Lauric acid
C14:0 - Myristic acid
C16:0 - Palmitic acid
C16:1 - Palmitoleic acid
C18:0 - Stearic acid
C18:1 - Oleic acid
C18:2 - Linoleic acid
C20:0 - Arachidic acid
C18:3 - Linolenic acid

(a) Unidentified: probably trans isomer and/or positional of C18:1

(b) Unidentified: probably trans isomer and/or positional of C18:2

(c) Unidentified

Softening points varied from 20.1°C to 58.4°C, for palm olein and hydrogenated palm oil, respectively. These values indicate a large range of melting point for the samples studied. This measurement was not done for soybean and cottonseed oils because this method does not apply to these samples due to their low melting points, -23 to -20°C for soybean oil and -2 to 2°C for cottonseed oil (Weiss, 1980)

Figures 1 to 14 show DSC melting curves obtained. Melting range and DSC curve shape result from combined effects between fatty acid composition, polymorphism and thermal history (Kaisersberger, 1989). Soybean oil has a characteristic curve about -25°C and its melting occurs at temperatures below 0°C (figure 1). In relation to hydrogenated soybean oils, there is a broadening of the curves and their moving to higher temperatures regions (figures 2 and 3). Formation of trans and positional isomers due to hydrogenation resulted in the formation of non-intersoluble triglycerides, increasing the melting range of the samples. The same phenomenon occurs with cottonseed oil and its hydrogenated and interesterified samples (figures 4, 5, and 6). Palm oil has a very characteristic curve, showing clearly its two component fractions, separated by an exothermic peak. (figure 7). Hydrogenated palm oil sample shows two peaks, corresponding to α and β polymorphic forms (figure 8). Palm olein (figure 9) shows only one peak, corresponding to the lowest temperature peak observed in palm oil while palm stearin (figure 10) shows a similar profile to that one of palm oil, showing two peaks. Palm kernel (figure 11) shows only one peak and a limited melting range. Palm kernel stearin (figure 12) has the same DSC profile of palm kernel, but its curve is sharper and is located at higher temperature, indicating a small melting range. Babassu oil (figure 13) has a similar profile of palm kernel oil, both with high concentrations of lauric acid (see table I). Hydrogenated babassu (figure 14) oil has a greater melting range, due to the formation of trans and positional isomers, as already commented about hydrogenated soybean and cottonseed oils.

Onset, peak temperatures and melting point temperatures obtained by DSC melting curves and AOCS Softening point values are shown in table II. When comparing DSC melting point values with softening point ones, those obtained by DSC technique are always higher than softening point ones, with differences ranging from 2.2 to 9.3°C, with average values of 5.2°C. Correlation between the temperatures obtained by the two techniques was calculated as 0.9856, considered high and indicating good relationship between the two techniques. These results agree with those obtained by Deman *et al.*, (1983) which compared Mettler dropping point and DSC melting points. DSC melting points were generally considerably higher than the Mettler dropping points.

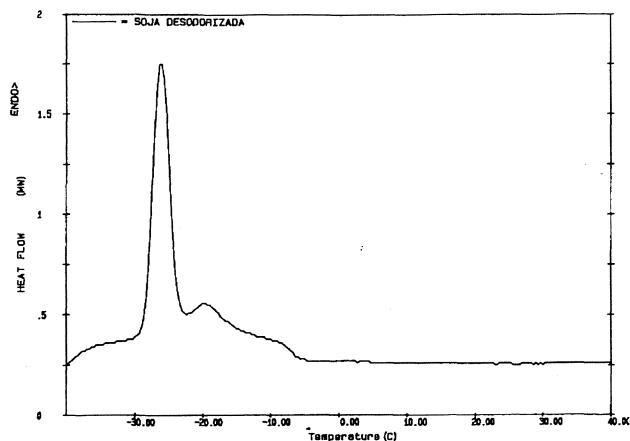


Figure 1
DSC melting curve for deodorized soybean oil

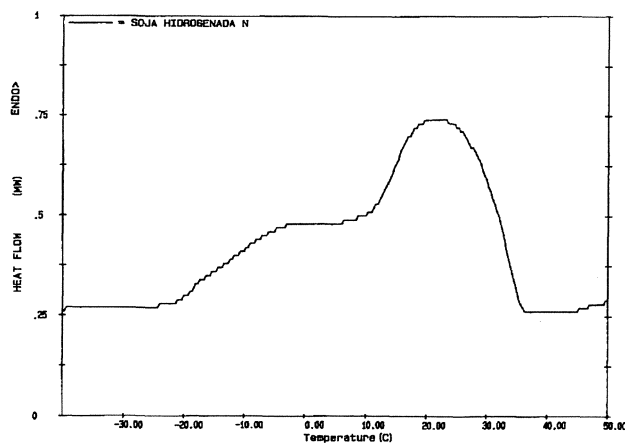


Figure 2
DSC melting curve for type «N» hydrogenated soybean oil

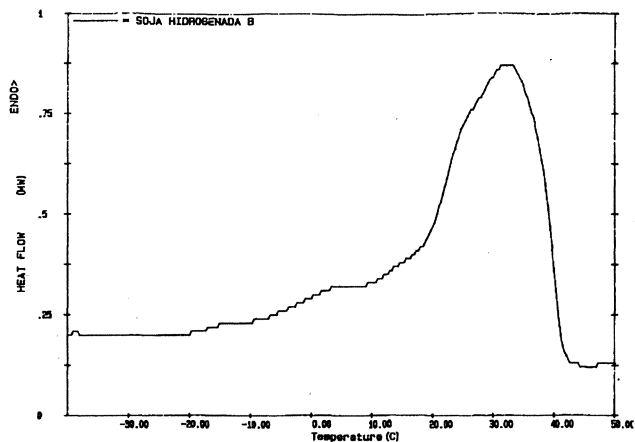


Figure 3
DSC melting curve for type «B» hydrogenated soybean oil

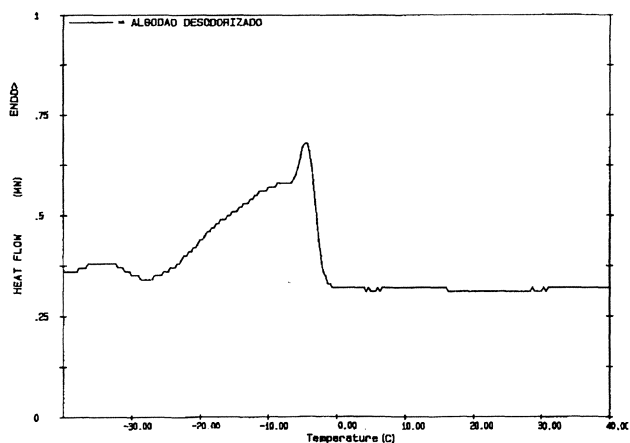


Figure 4
DSC melting curve for deodorized cottonseed oil

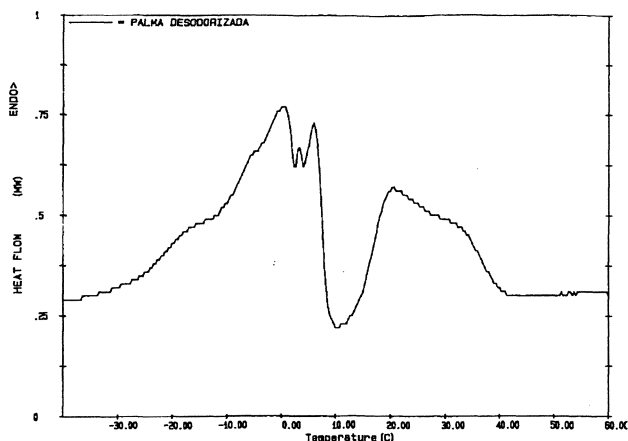


Figure 7
DSC melting curve for deodorized palm oil

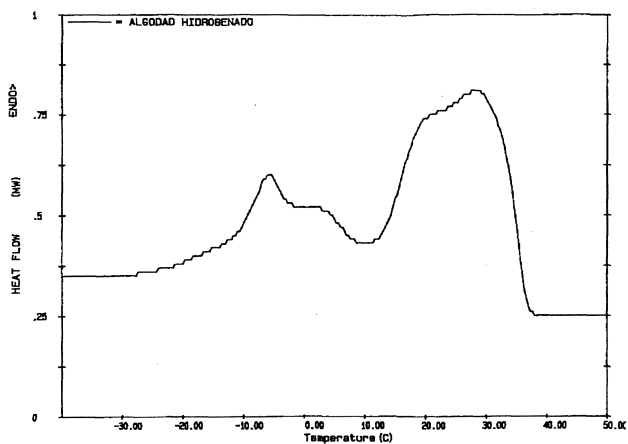


Figure 5
DSC melting curve for hydrogenated cottonseed oil

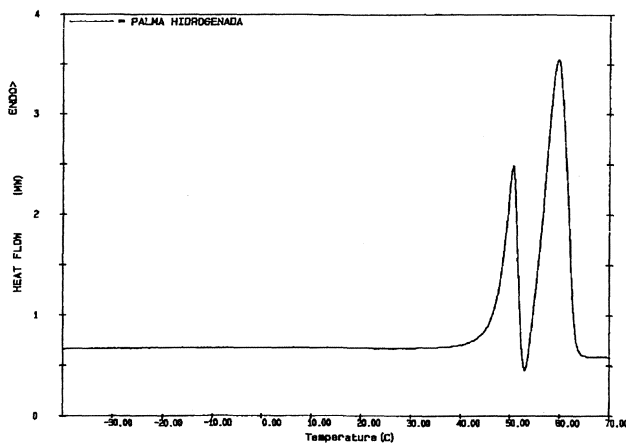


Figure 8
DSC melting curve for hydrogenated palm oil

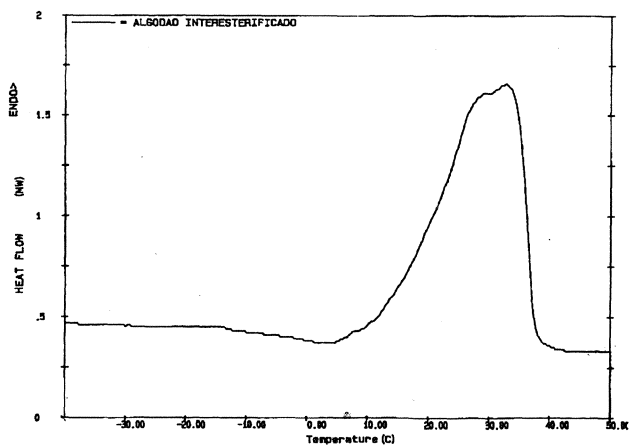


Figure 6
DSC melting curve for interesterified cottonseed oil

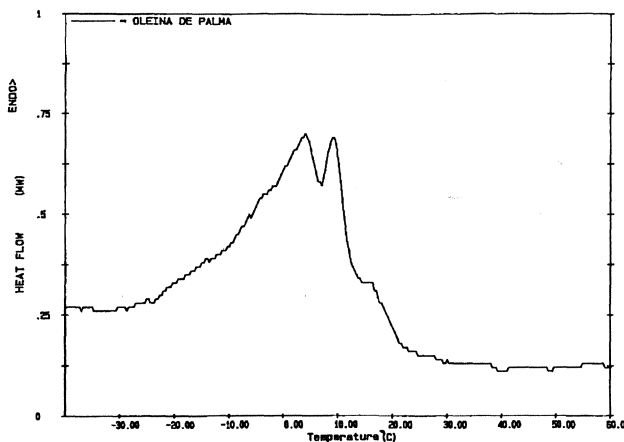


Figure 9
DSC melting curve for palm oil

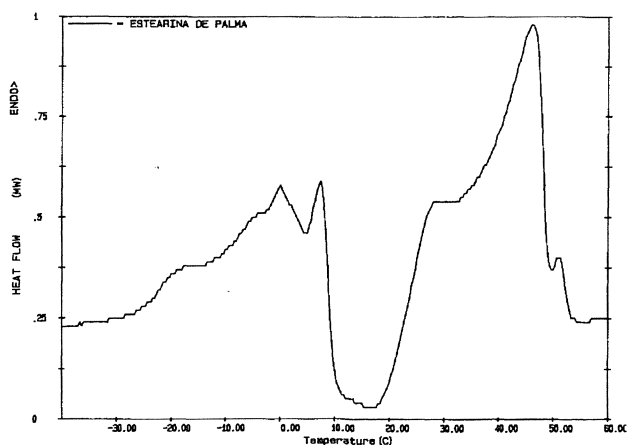


Figure 10
DSC melting curve for palm stearin

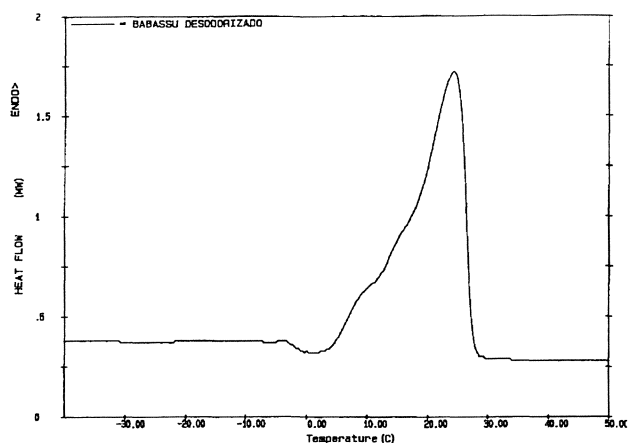


Figure 13
DSC melting curve for deodorized babassu oil

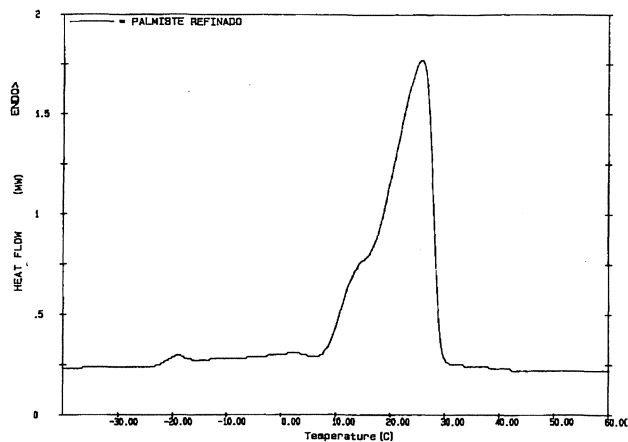


Figure 11
DSC melting curve for refined palm kernel oil

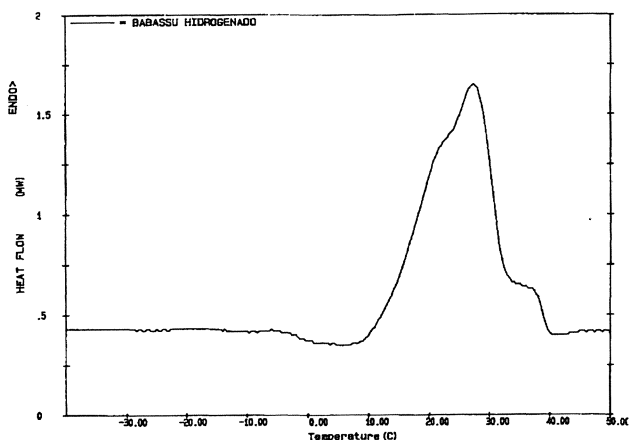


Figure 14
DSC melting curve for hydrogenated babassu oil

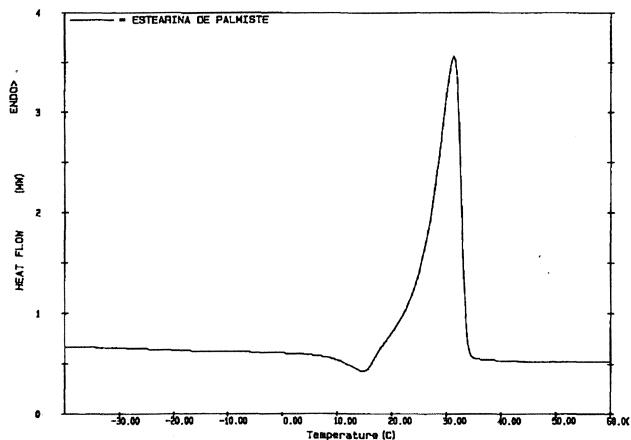


Figure 12
DSC melting curve for palm kernel stearin

Figure 15 shows a graphical comparison between differences of melting points and other characteristic temperatures obtained by DSC melting curves and softening point values. If onset temperatures were considered, differences between these temperatures and softening point ones are bigger, because onset temperatures were recorded when the fat began to melt, while in softening point they had melted more than this point recorded by DSC. When comparing peak temperatures obtained by DSC with softening points, we can observe that the former are higher than those obtained by DSC, except for hydrogenated palm sample. Big differences can be seen between deodorized palm oil and palm olein. This fact occurs because peak temperature is recorded as the temperature of the main peak, when curve shows more than one. In this case, main peak of both samples was located in a region where temperature was not sufficient to melt the sample in the same point of that recorded by softening point.

Explore Litigation Insights

Docket Alarm provides insights to develop a more informed litigation strategy and the peace of mind of knowing you're on top of things.

Real-Time Litigation Alerts



Keep your litigation team up-to-date with **real-time alerts** and advanced team management tools built for the enterprise, all while greatly reducing PACER spend.

Our comprehensive service means we can handle Federal, State, and Administrative courts across the country.

Advanced Docket Research



With over 230 million records, Docket Alarm's cloud-native docket research platform finds what other services can't. Coverage includes Federal, State, plus PTAB, TTAB, ITC and NLRB decisions, all in one place.

Identify arguments that have been successful in the past with full text, pinpoint searching. Link to case law cited within any court document via Fastcase.

Analytics At Your Fingertips



Learn what happened the last time a particular judge, opposing counsel or company faced cases similar to yours.

Advanced out-of-the-box PTAB and TTAB analytics are always at your fingertips.

API

Docket Alarm offers a powerful API (application programming interface) to developers that want to integrate case filings into their apps.

LAW FIRMS

Build custom dashboards for your attorneys and clients with live data direct from the court.

Automate many repetitive legal tasks like conflict checks, document management, and marketing.

FINANCIAL INSTITUTIONS

Litigation and bankruptcy checks for companies and debtors.

E-DISCOVERY AND LEGAL VENDORS

Sync your system to PACER to automate legal marketing.