

USP 24

THE UNITED STATES PHARMACOPEIA

NF 19

THE NATIONAL FORMULARY

By authority of the United States Pharmacopeial Convention, Inc., meeting at Washington, D.C., March 9–12, 1995. Prepared by the Committee of Revision and published by the Board of Trustees

Official from January 1, 2000


UNITED STATES PHARMACOPEIAL CONVENTION, INC.
12601 Twinbrook Parkway, Rockville, MD 20852

Argentum EX1040

determination, and make any necessary corrections.

METHOD II (AZEOTROPIC—TOLUENE DISTILLATION)

Apparatus—Use a 500-mL glass flask *A* connected by means of a trap *B* to a reflux condenser *C* by ground glass joints (see figure).

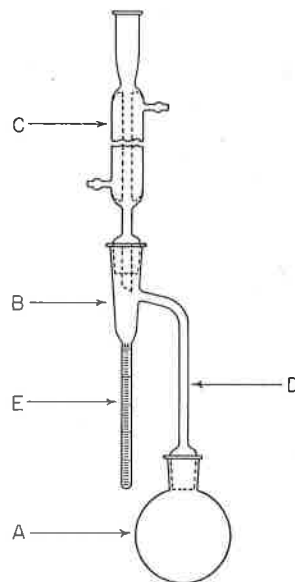

Toluene Moisture Apparatus

The critical dimensions of the parts of the apparatus are as follows. The connecting tube *D* is 9 to 11 mm in internal diameter. The trap is 235 to 240 mm in length. The condenser, if of the straight-tube type, is approximately 400 mm in length and not less than 8 mm in bore diameter. The receiving tube *E* has a 5-mL capacity, and its cylindrical portion, 146 to 156 mm in length, is graduated in 0.1-mL subdivisions, so that the error of reading is not greater than 0.05 mL for any indicated volume. The source of heat is preferably an electric heater with rheostat control or an oil bath. The upper portion of the flask and the connecting tube may be insulated.

Clean the receiving tube and the condenser with chromic acid cleansing mixture, thoroughly rinse with water, and dry in an oven. Prepare the toluene to be used by first shaking with a small quantity of water, separating the excess water, and distilling the toluene.

Procedure—Place in the dry flask a quantity of the substance, weighed accurately to the nearest centigram, which is expected to yield 2 to 4 mL of water. If the substance is of a pasty character,

of water adhere to the walls of the receiving tube, scrub them with a brush consisting of a rubber band wrapped around a wire and wetted with toluene. When the water and toluene separated completely, read the volume of water, and calculate percentage that was present in the substance.

METHOD III (GRAVIMETRIC)

Procedure for Chemicals—Proceed as directed in the individual monograph preparing the chemical as directed under *Loss on Drying* (731).

Procedure for Biologics—Proceed as directed in the individual monograph.

Procedure for Vegetable Drugs—Place about 10 g of the substance to be prepared as directed (see *Vegetable Drugs—Methods of Analysis* (561)) and accurately weighed, in a tared evaporating dish. Immerse in a water bath at 105° for 5 hours, and weigh. Continue the drying and weighing at 1-hour intervals until the difference between two successive weighings corresponds to not more than 0.25%.

(941) X-RAY DIFFRACTION

Every crystal form of a compound produces its own characteristic X-ray diffraction pattern. These diffraction patterns can be determined either from a single crystal or from a powdered specimen (consisting of numerous crystals) of the material. The spacings between the diffraction maxima can be used for the qualitative and quantitative analysis of crystalline materials. Powder diffraction techniques are most commonly employed for the identification and the determination of relative purity of crystalline materials. Small amounts of impurity, however, are not normally detectable by the X-ray diffraction method, and for quantitative measurements it is necessary to prepare the sample carefully to avoid preferred orientation effects.

The powder methods provide an advantage over other methods of analysis in that they are usually nondestructive in nature (specimen preparation is usually limited to grinding to ensure a random oriented sample, and deleterious effects of X-rays on solid pharmaceutical compounds are not commonly encountered). The primary use of single-crystal diffraction data is for the determination of molecular weights and analysis of crystal structures at the atomic level. However, diffraction data established for a single crystal can be used to support a specific powder pattern as being truly representative of the single phase.

Solids—A solid substance can be classified as being crystalline, noncrystalline, or a mixture of the two forms. In crystalline materials, the molecular or atomic species are ordered in a three-dimensional array, called a lattice, within the solid particles. This order of molecular components is lacking in noncrystalline material. Crystalline solids sometimes are referred to as glasses or amorphous solids when repetitive order is nonexistent in all three dimensions. It is also possible for order to exist in only one or two dimensions, resulting in mesomorphic phases (liquid crystals). Although crystalline materials are usually considered to have well-defined external morphologies (their habits), this is not a necessity for X-ray diffraction analysis.

The relatively random arrangement of molecules in noncrystalline substances makes them poor coherent scatterers of X-rays, resulting in broad, diffuse maxima in diffraction patterns. The

acteristic X-ray patterns, so does every solvate. Sometimes the differences in the diffraction patterns of different polymorphs are relatively minor, and must be very carefully evaluated before a definitive conclusion is reached. In some instances, these polymorphs and / or solvates show varying dissolution rates. Therefore, on the time scale of pharmaceutical bioavailability, different total amounts of drug are dissolved, resulting in potential bioinequivalence of the several forms of the drug.

Fundamental Principles—A collimated beam of monochromatic X-rays is diffracted in various directions when it impinges upon a rotating crystal or randomly oriented powdered crystal. The crystal acts as a three-dimensional diffraction grating to this radiation. This phenomenon is described by Bragg's law, which states that diffraction (constructive interference) can occur only when waves that are scattered from different regions of the crystal, in a specific direction, travel distances differing by integral numbers (n) of the wavelength (λ). Under such circumstances, the waves are in phase. This condition is described by the Bragg equation:

$$\frac{n\lambda}{2 \sin \theta} = d_{hkl}$$



in which d_{hkl} denotes the interplanar spacings and θ is the angle of diffraction.

A family of planes in space can be indexed by three whole numbers, usually referred to as Miller indices. These indices are the reciprocals, reduced to smallest integers, of the intercepts that a plane makes along the axes corresponding to three nonparallel edges of the unit cell (basic crystallographic unit). The unit cell dimensions are given by the lengths of the spacings along the three axes, a , b , c , and the angles between them, α , β , and γ . The interplanar spacing for a specific set of parallel planes hkl is denoted by d_{hkl} . Each such family of planes may show higher orders of diffraction where the d values for the related families of planes nh , nk , nl are diminished by the factor $1/n$ (n being an integer: 2, 3, 4, etc.). Every set of planes throughout a crystal has a corresponding Bragg diffraction angle associated with it (for a specific λ).


The amplitude of a diffracted X-ray beam from any set of planes is dependent upon the following atomic properties of the crystal: (1) position of each atom in the unit cell; (2) the respective atomic scattering factors; and (3) the individual thermal motions. Other factors that directly influence the intensities of the diffracted beam are: (1) the intensity and wavelength of the incident radiation; (2) the volume of crystalline specimen; (3) the absorption of the X-radiation by the specimen; and (4) the experimental arrangement utilized to record the intensity data. Thus, the experimental conditions are especially important for measurement of diffraction intensities.

Only a limited number of Bragg planes are in a position to diffract when monochromatized X-rays pass through a single crystal. Techniques of recording the intensities of all of the possible diffracting hkl planes involve motion of the single crystal and the recording media. Recording of these data is accomplished by photographic techniques (film) or with radiation detectors.


A beam passing through a very large number of small, randomly oriented crystals produces continuous cones of diffracted rays from each set of lattice planes. Each cone corresponds to the diffraction from various planes having a similar interplanar spacing. The intensities of these Bragg reflections are recorded by either film or radiation detectors. The Bragg angle can be measured easily from a film, but the advent of radiation detectors has made possible the construction of diffractometers that read this angle directly. The intensities and d spacings are more conveniently determined with powder diffractometers employing radiation detectors than by film

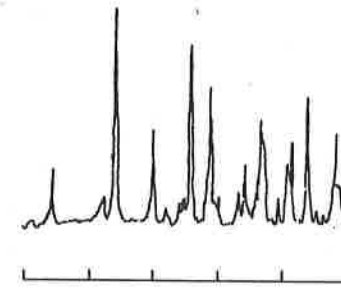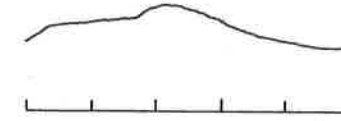

Trihydrate

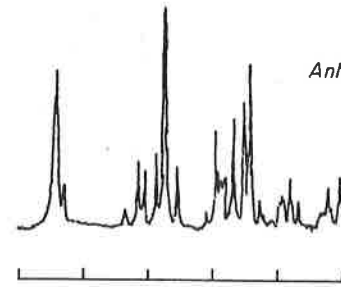

Anhydrous form 1

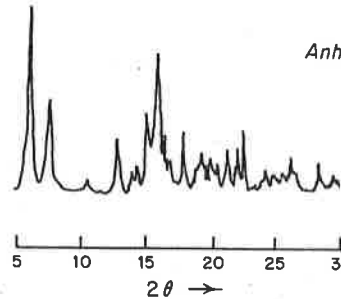

Anhydrous form 2

5 10 15 20 25 30
2θ →

Typical Powder Patterns Obtained for Four Solid Phases of Ampicillin

Radiation—The principal radiation sources utilized for X-ray diffraction are vacuum tubes utilizing copper, molybdenum, iron, and chromium as anodes; copper X-rays are employed most commonly for organic substances. For each of these radiations there is an element that will filter off the $K\beta$ radiation and permit the $K\alpha$ radiation to pass (nickel is used, in the case of copper radiation). In this manner the radiation is practically monochromatized. The choice of radiation to be used depends upon the absorption characteristics of the material and possible fluorescence by atoms present in the specimen.

sities of various reflections.

Several specialized handling techniques may be employed to minimize preferred orientation, but further reduction of particle size is often the best approach.

Where very accurate measurement of the Bragg angles is necessary, a small amount of an internal standard can be mixed into the specimen. This enables the film or recorder tracing to be calibrated. If comparisons to literature values (including compendial limits) of d are being made, calibrate the diffractometer. NIST standards are available covering to a d -value of 0.998 nm. Tetradecanol¹ may be used (d is 3.963 nm) for larger spacing.

The absorption of the radiation by any specimen is determined by the number and kinds of atoms through which the X-ray beam passes. An organic matrix usually absorbs less of the diffracted radiation than does an inorganic matrix. Therefore, it is important in quantitative studies that standard curves relating amount of material to the intensity of certain d spacings for that substance be

¹ Brindley, GW and Brown, G, eds., *Crystal Structures of Clay Minerals and their X-ray Identification*, Mineralogical Society Monograph No. 5, London, 1980, pp. 318 ff.

known materials with those of the unknown. The intensity (ratio of the peak intensity of a particular d spacing to the intensity of the strongest maxima in the diffraction pattern) and the d spacing are used in the comparison. If a reference material (e.g., US Reference Standard) is available, it is preferable to generate a preferred reference pattern on the same equipment used for running the known sample, and under the same conditions. For most organic crystals, it is appropriate to record the diffraction pattern in the 2θ region from as near zero degrees as possible to 40 degrees. Agreement between sample and reference should be within the calibrated precision of the diffractometer for diffraction angles (2θ values should typically be reproducible to ± 0.10 degrees), while relative intensities between sample and reference may vary considerably. For other types of samples (e.g., inorganic salts), it may be necessary to extend the 2θ region scanned to beyond 40 degrees. It is generally sufficient to scan past the strongest reflections identified in the Powder Diffraction File

² The International Centre for Diffraction Data, Newtown Square Corporate Campus, 12 Campus Boulevard, Newtown Square, PA 19073, maintains a file on more than 60,000 crystalline materials, both organic and inorganic, suitable for such comparisons.

U. S. PHARMACOPEIA

NATIONAL FORMULARY

USP 23

NE 18

Explore Litigation Insights

Docket Alarm provides insights to develop a more informed litigation strategy and the peace of mind of knowing you're on top of things.

Real-Time Litigation Alerts



Keep your litigation team up-to-date with **real-time alerts** and advanced team management tools built for the enterprise, all while greatly reducing PACER spend.

Our comprehensive service means we can handle Federal, State, and Administrative courts across the country.

Advanced Docket Research



With over 230 million records, Docket Alarm's cloud-native docket research platform finds what other services can't. Coverage includes Federal, State, plus PTAB, TTAB, ITC and NLRB decisions, all in one place.

Identify arguments that have been successful in the past with full text, pinpoint searching. Link to case law cited within any court document via Fastcase.

Analytics At Your Fingertips



Learn what happened the last time a particular judge, opposing counsel or company faced cases similar to yours.

Advanced out-of-the-box PTAB and TTAB analytics are always at your fingertips.

API

Docket Alarm offers a powerful API (application programming interface) to developers that want to integrate case filings into their apps.

LAW FIRMS

Build custom dashboards for your attorneys and clients with live data direct from the court.

Automate many repetitive legal tasks like conflict checks, document management, and marketing.

FINANCIAL INSTITUTIONS

Litigation and bankruptcy checks for companies and debtors.

E-DISCOVERY AND LEGAL VENDORS

Sync your system to PACER to automate legal marketing.