

RESEARCH ARTICLE

Open Access



Changes in views on digital intraoral scanners among dental hygienists after training in digital impression taking

Hye-Ran Park¹, Ji-Man Park², Youn-Sic Chun³, Kkot-Nim Lee¹ and Minji Kim^{3*}

Abstract

Backgrounds: Despite the rapid development of digital dentistry, the use of digital intraoral scanners remains limited. The aim of this study was to evaluate the changes in views on intraoral scanners among dental hygienists after training.

Methods: Thirty-four dental hygienists with >3 years of clinical experience participated and were divided into 2 groups: iTero and Trios groups. Participants of each group practiced the usage of both intraoral scanners, for total 12 times over 4 sessions. Questionnaires were given to participants at two different times; prior to and after the completion of the training sessions. The parameters of questionnaires included on difficulty of use, patient discomfort, awareness, preference, and clinical usefulness of intraoral scanners and comparison of two types of scanners.

Results: Upon the completion of the training, both iTero and Trios groups gave positive feedback on anticipated accuracy, efficiency, and clinical usefulness. More participants of the iTero group responded that the level of difficulty of use and patient discomfort was greater than Trios. Both groups preferred Trios for its clinical usefulness.

Conclusions: The perceptions of dental hygienists on usage of intraoral scanner and digital impression improved positively with the training. The participants favored Trios over iTero in terms of difficulty of use, patient comfort, and clinical usefulness. This study showed that appropriate training could change the views on the efficiency of intraoral scanners positively among dental hygienists.

Keywords: Digital intraoral scanner, Perception of digital impression, Training of intraoral scanner

Backgrounds

Computer-aided design/computer-aided manufacture (CAD/CAM) was first introduced in the field of dentistry in the 1980s; since then, the use of digital technology has been rapidly increased in dentistry, though having some arguments on its accuracy [1–4]. The conventional impression-taking method may pose patient discomfort and possibility of deformation which could be affected by the type of impression material [5–9], impression tray [10–12], and impression technique [13]. The digital impression technique could overcome these limitations by providing simple operating system [2, 14], accuracy, and improved patient comfort [15, 16]. Additional advantages

include providing a preview of three-dimensional (3D) images while taking the impression. Some studies evaluated on accuracy of digital impression technique using intraoral scanners and reported that accuracy could be affected by materials or scanning strategies [2, 4]. Previous studies on the digital impression-taking using intraoral scanners have been limited to the accuracy and efficiency of intraoral scanners [17–19]. Some of previous studies compared the inconvenience and difficulty of digital impression method using between intraoral scanners compared to conventional impression methods among dental students in the university [15, 20, 21]. The aim of this study is to evaluate the changes in views on intraoral scanners among dental hygienists after training in digital impression.

* Correspondence: minjikim@ewha.ac.kr

³Department of Orthodontics, Graduate School of Clinical Dentistry, Ewha Womans University, 1071, Anyangcheon-ro, Yangcheon-gu, Mokdong Hospital, Seoul, Korea

Full list of author information is available at the end of the article



© 2015 Park et al. **Open Access** This article is distributed under the terms of the Creative Commons Attribution 4.0 International License (<http://creativecommons.org/licenses/by/4.0/>), which permits unrestricted use, distribution, and reproduction in any medium, provided you give appropriate credit to the original author(s) and the source, provide a link to the Creative Commons license, and indicate if changes were made. The Creative Commons Public Domain Dedication waiver (<http://creativecommons.org/publicdomain/zero/1.0/>) applies to the data made available in this article, unless otherwise stated.

Methods

Participants

Thirty-four dental hygienists with a clinical experience of at least 3 years who had no experience in using intraoral scanners participated in the study and they were divided into 2 groups ; an iTero (n = 17) and a Trios (n = 17) group using random allocation method. All participants were recruited voluntarily after the informative session about the study and written consent forms were obtained. This study was approved by the Institutional Review Board Committee of Ewha Womans University Medical College (Approval number: ECT14-02A-27).

Intraoral scanners

In this study, 2 different types of 3D intraoral scanners, iTero® (Align Technology Inc. Santa Clara, California) and Trios® (3Shape dental systems, Copenhagen, Denmark), were used. The iTero is operated by the parallel confocal principle and acquires 3D data by over 100,000 red laser beams to the object and fusing the acquired images. The weight of the wand is 1,100 g. The Trios is operated by the confocal principle with the video-recording method based on the real-time rendering technique. The scanner head of Trios weighs 760 g. Both intraoral scanners were operated according to the manufacturer’s instructions.

Study design and Workflow

All participants not only performed as operators, but also underwent to have scanning experience as patients. The participants were fully trained with only one scanner according to assigned group, and the other scanner

was used once for the comparing purpose between two different scanners. On the first day, each group of participants filled out the first questionnaire before the training was initiated. Then, the principles and operational concepts of iTero and Trios intraoral scanner devices were introduced. Practice session of intraoral scanner on models was followed by actual intraoral scanning activity. Digital impression from actual intraoral scan was obtained twice. On the second day, each group of participants practiced and took intraoral digital impression for three times. And all participants also underwent for iTero scanning experience as patients, which was operated by a qualified professional. On the third day, all participants again acquired actual intraoral images for 3 times. And they underwent Trios scanning experience as patients, which was operated by a qualified professional. On the last day, all participants acquired actual intraoral digital impression for twice and then practiced once on models again. Finally, each group of participants exchanged to the other scanner and acquired digital impression once intraorally. Upon the completion of the training sessions, all participants completed the second questionnaire.(Fig. 1)

Questionnaire configuration

Two questionnaires were administered during the study (Additional file 1). The first preliminary questionnaire was given initially before the training sessions and the second questionnaire was completed upon the completion of all the training sessions. The first questionnaire was administered before the training sessions and evaluated three




Fig. 1 Procedure workflow

main parameters: difficulties of using intraoral scanners with digital impression method compared to conventional impression-taking method, patient comfort, and degree of awareness about intraoral scanners. The parameter of awareness included anticipated accuracy, patient convenience, efficiency, clinical application, and interest in further use. The second questionnaire was administered upon the completion of all the training sessions and evaluated all the above parameters in addition to parameters of preference, clinical usefulness, and comparison of the two different types of scanners.

Statistical analysis

All statistical analyses were performed using IBM Statics 19.0 (SPSS Inc., Chicago, USA) software. The paired t-test was used to test differences. The level of significance was set at 0.05.

Results

Views on difficulty of use and patient comfort before and after training

There was no significant difference in views on difficulties of using intraoral scanner devices for digital impression-taking method compared to that with conventional impression-taking methods before and after training in both the iTero and Trios groups (Table 1). A similar result was shown for parameter of patient comfort.

In the iTero group, prior to the training sessions, 53 % of participants responded that digital impression taking method may be easier than taking conventional impression using rubber materials. However, after the training sessions, only 24 % of participants in iTero group responded that digital impression taking method may be easier compared to conventional rubber impression taking method (Fig. 2). In the Trios group, the response rate for the same question was 47 %, prior to and after the training. Furthermore, when the difficulties of using digital impression taking method was compared to the conventional impression taking method using alginate material the participants responded digital impression to be more difficult as 71 % and 82 % before and after training,

respectively, in the iTero group, and 65 % and 53 % before and after training, respectively, in the Trios group.

To evaluate parameter of patient comfort, all the participants underwent digital impression scanning experience using iTero and Trios. Before the training, 65 % of participants in the iTero group and 41 % of participants in the Trios group responded that digital impression taking may be more comfortable to patients than impression taking using rubber materials; these rates decreased to 53 % in the iTero group and increased to 47 % in the Trios group. In comparison with patient comfort during impression taking using alginate, subjects who answered that digital impression taking was more convenient decreased from 53 % to 41 % in the iTero group and remained the same in the Trios group (53 %).

The number of subjects who responded that digital impression taking was easier than conventional impression taking as an operator was greater for rubber impression materials than for alginate. This was due to difficulty, and higher level of expected precision in the use of rubber materials. The number of responses that digital impression taking was more difficult generally increased after training in the iTero group and decreased in the Trios group. With regard to patient comfort, the number of responses that digital impression taking was more convenient was almost similar before and after training in both groups.

Awareness about digital impression taking before and after training

As shown in Table 2, scores for the anticipated accuracy of digital impression taking method increased after the training in the iTero group. With regard to clinical usefulness, after the training sessions, more participants in the iTero group answered that digital scanners could be helpful tools in dental clinics. However, there were no significant differences for other parameters before and after training in the iTero group. In the Trios group, there were no significant differences for any parameters.

The participants from both groups generally showed positive responses for all parameters of digital impression taking method (Fig. 3).

Table 1 Difficulty of use and patient discomfort while using intraoral scanners and rubber and alginate materials, before and after training (10-point Likert scale)

Variables	Conventional impression material	iTero group		p-value	Trios group		p-value
		Mean (SD)			Mean (SD)	Mean (SD)	
		Before	After		Before	After	
Level of difficulty	Rubber	4.65 (2.09)	5.65 (1.94)	.101	5.12 (1.80)	5.00 (2.26)	.847
	Alginate	6.18 (2.38)	7.29 (1.65)	.128	5.77 (2.46)	5.59 (2.62)	.779
Level of Patient discomfort	Rubber	4.29 (2.05)	4.12 (1.83)	.726	4.47 (2.63)	4.47 (2.79)	1.000
	Alginate	4.88 (2.29)	5.18 (2.33)	.663	4.24 (2.10)	4.47 (2.76)	.680

10-point Likert scale: 0 ~ 4 = low score (Digital impression taking was easier and more convenient) 5; neutral; 6 ~ 10 = high score (Digital impression taking was difficult and inconvenient)




Fig. 2 Difficulty of use and patient inconvenience between intraoral scanners and rubber and alginate materials before and after training (10-point Likert scale)

Preference for digital impression taking

As shown in Fig. 4, all participants from both groups gave a positive overall feedbacks for digital impression taking method. The results showed that 82.4 % participants of both iTero and Trios groups showed willingness to use the intraoral scanner in the future. Participants agreed that the training for the intraoral scanner is useful; 94.1 %

participants in the iTero group and 88.2 % participants in the Trios group. All subjects were interested in receiving information about intraoral scanners.


Views on clinical usefulness in the iTero and Trios groups

In terms of the subjective weight of the scanner head between two intraoral scanners, in the iTero group, the

Table 2 Awareness about digital impression taking before and after training (7-point Likert scale)

Parameters	Variables (Scores for agreement regarding digital impression taking)	iTero			Trios		
		Mean (SD)		p-value	Mean (SD)		p-value
		Before	After		Before	After	
Accuracy	More accurate than rubber impression taking	4.29 (1.45)	4.82 (1.24)	0.024*	5.06 (1.09)	5.59 (1.23)	0.132
	More accurate than alginate impression taking	4.77 (1.60)	5.35 (1.62)	0.096	5.47 (1.13)	6.06 (1.09)	0.086
Convenience	More efficient management of impression model	5.88 (1.69)	6.29 (1.49)	0.130	6.41 (0.80)	6.59 (0.62)	0.484
Efficiency	Possibility of saving time compared to rubber impressions	5.24 (1.60)	4.88 (1.57)	0.455	4.65 (1.54)	4.82 (1.63)	0.661
	Possibility of saving time compared to alginate impressions	4.29 (2.14)	4.06 (2.05)	0.702	4.29 (1.72)	4.06 (1.78)	0.632
	Influence on simplification of the entire treatment process	5.24 (1.03)	5.06 (1.56)	0.627	5.18 (1.01)	5.47 (1.06)	0.311
	Usefulness in attracting patient’s attention.	5.82 (1.43)	6.12 (0.78)	0.385	5.47 (1.18)	6.00 (0.94)	0.083
Clinical usefulness	Influence on increasing patient’s trust.	5.35 (1.58)	5.88 (0.78)	0.120	5.59 (1.06)	5.77 (0.90)	0.616
	Influence on promoting the dental clinic.	5.35 (1.50)	5.88 (0.99)	0.034*	5.59 (1.06)	6.00 (0.87)	0.069
Skill acquisition	Ease of training in a short time	4.47 (1.28)	4.06 (1.30)	0.370	4.65 (1.46)	4.65 (1.73)	1.000
	Effect of proficiency in using digital impression techniques on the accuracy	6.24 (0.83)	6.59 (0.71)	0.251	6.18 (0.88)	6.18 (0.72)	1.000
	Superior ability in taking digital impressions compared to other colleagues	5.18 (1.33)	5.41 (1.27)	0.299	5.65 (1.00)	5.71 (0.85)	0.817
	Usefulness of digital impression in the clinical environment	4.82 (1.28)	5.18 (1.29)	0.370	5.47 (0.80)	5.53 (1.23)	0.848
	Positive interest in taking digital impressions	5.59 (1.06)	5.29 (0.92)	0.206	5.65 (0.79)	5.71 (1.11)	0.848

7-point Likert scale: 1 = very strongly disagree, 2 = strongly disagree, 3 = disagree, 4 = neutral, 5 = agree, 6 = strongly agree, 7 = very strongly agree, *: p < 0.05

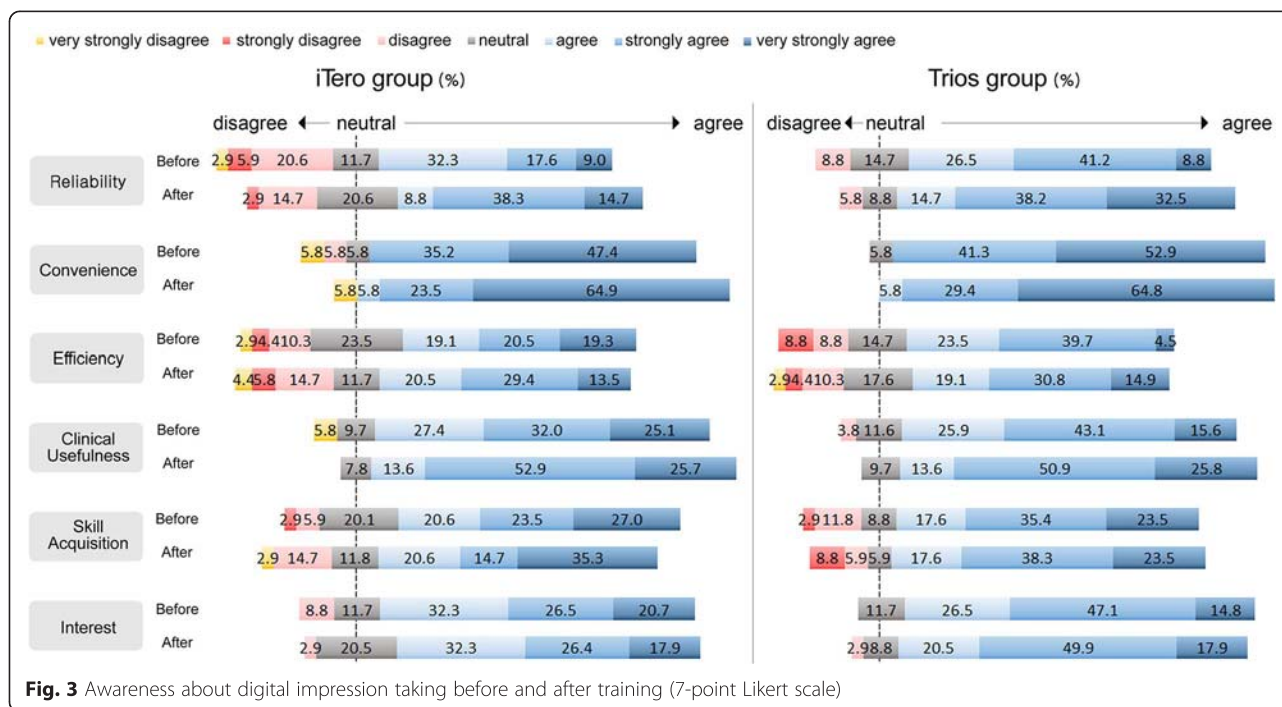


degree of agreement to the fact that the scanner head was light was significantly higher for Trios (2.65 ± 0.86) than for iTero (1.65 ± 0.78) (Table 3). Similar results were shown in Trios group. In the iTero group, the response that handling the scanner was convenient showed a significantly different degree of agreement for iTero (2.52 ± 0.87) and Trios (3.17 ± 0.52). With regard to the ease of software and hardware operation in the Trios group, more respondents agreed that Trios was easy to operate.

These results suggested that positive responses for clinical usefulness were greater with Trios than for iTero intraoral scanner.

Views on difficulty of use and patient comfort in the iTero and Trios groups

As shown as Table 4, in the iTero group, the level of difficulty of use was rated higher for iTero (5.47 ± 2.37) than for Trios (4.23 ± 1.92), as was the level of

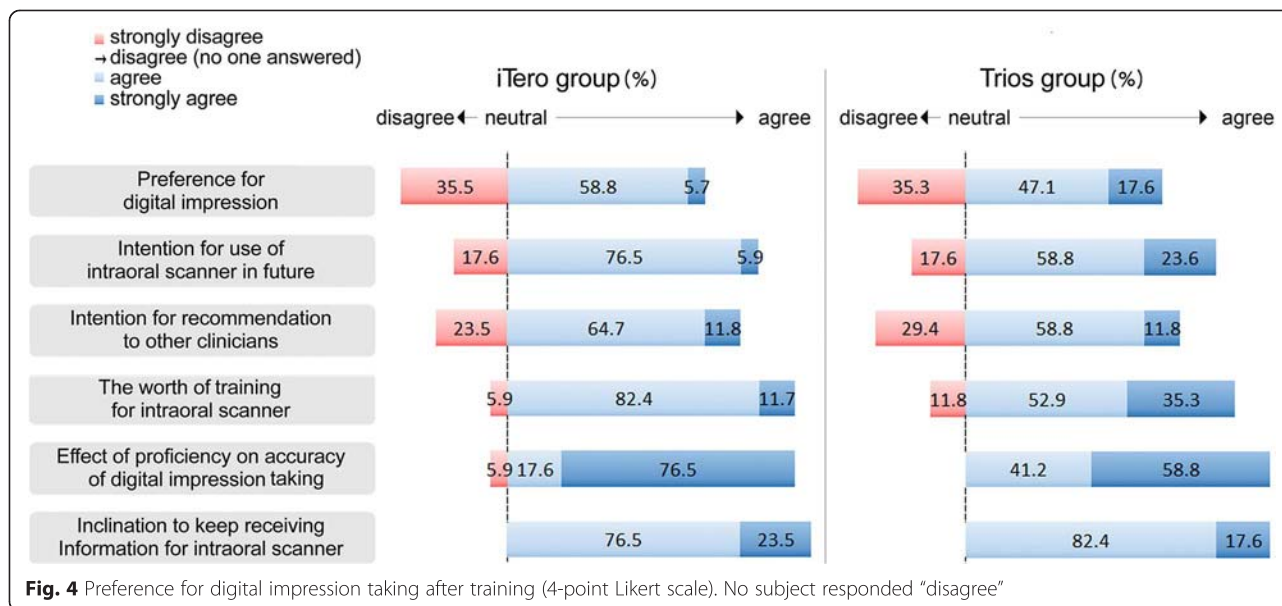

Explore Litigation Insights

Docket Alarm provides insights to develop a more informed litigation strategy and the peace of mind of knowing you're on top of things.

Real-Time Litigation Alerts



Keep your litigation team up-to-date with **real-time alerts** and advanced team management tools built for the enterprise, all while greatly reducing PACER spend.

Our comprehensive service means we can handle Federal, State, and Administrative courts across the country.

Advanced Docket Research



With over 230 million records, Docket Alarm's cloud-native docket research platform finds what other services can't. Coverage includes Federal, State, plus PTAB, TTAB, ITC and NLRB decisions, all in one place.

Identify arguments that have been successful in the past with full text, pinpoint searching. Link to case law cited within any court document via Fastcase.

Analytics At Your Fingertips



Learn what happened the last time a particular judge, opposing counsel or company faced cases similar to yours.

Advanced out-of-the-box PTAB and TTAB analytics are always at your fingertips.

API

Docket Alarm offers a powerful API (application programming interface) to developers that want to integrate case filings into their apps.

LAW FIRMS

Build custom dashboards for your attorneys and clients with live data direct from the court.

Automate many repetitive legal tasks like conflict checks, document management, and marketing.

FINANCIAL INSTITUTIONS

Litigation and bankruptcy checks for companies and debtors.

E-DISCOVERY AND LEGAL VENDORS

Sync your system to PACER to automate legal marketing.