



US009241676B2

(12) **United States Patent**
Lisogurski et al.

(10) **Patent No.:** **US 9,241,676 B2**
(45) **Date of Patent:** ***Jan. 26, 2016**

(54) **METHODS AND SYSTEMS FOR POWER OPTIMIZATION IN A MEDICAL DEVICE**

(75) Inventors: **Daniel Lisogurski**, Boulder, CO (US);
Clark R. Baker, Jr., Newman, CA (US)

(73) Assignee: **Covidien LP**, Mansfield, MA (US)

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 128 days.

This patent is subject to a terminal disclaimer.

(21) Appl. No.: **13/484,770**

(22) Filed: **May 31, 2012**

(65) **Prior Publication Data**

US 2013/0324856 A1 Dec. 5, 2013

(51) **Int. Cl.**

A61B 5/00 (2006.01)
A61B 5/021 (2006.01)
A61B 5/024 (2006.01)
A61B 5/1455 (2006.01)

(52) **U.S. Cl.**

CPC **A61B 5/7285** (2013.01); **A61B 5/021** (2013.01); **A61B 5/02416** (2013.01); **A61B 5/02433** (2013.01); **A61B 5/14551** (2013.01)

(58) **Field of Classification Search**

CPC **A61B 5/021**; **A61B 5/02416**; **A61B 5/14551**; **A61B 5/7285**
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

5,343,818 A 9/1994 McCarthy et al.
5,349,952 A 9/1994 McCarthy et al.
5,351,685 A 10/1994 Potratz

5,485,847 A 1/1996 Baker, Jr.
5,515,847 A 5/1996 Braig et al.
5,560,355 A 10/1996 Merchant et al.
5,575,284 A 11/1996 Athan et al.
5,590,652 A 1/1997 Inai
5,746,697 A 5/1998 Swedlow et al.
5,766,127 A 6/1998 Pologe et al.
5,846,190 A 12/1998 Woehrl
5,924,979 A 7/1999 Swedlow et al.
6,005,658 A 12/1999 Kaluza et al.

(Continued)

FOREIGN PATENT DOCUMENTS

WO WO 2006/080856 8/2006
WO WO 2006/083180 8/2006

OTHER PUBLICATIONS

Takada, H. et al., "Acceleration Plethysmography to Evaluate Aging Effect in Cardiovascular System," Medical Progress Through Technology, vol. 21, pp. 205-210, 1997.

(Continued)


Primary Examiner — Mark Remaly

(74) *Attorney, Agent, or Firm* — Shvarts & Leiz LLP

(57) **ABSTRACT**

A physiological monitoring system may use photonic signals to determine physiological parameters. The system may vary parameters of a light drive signal used to generate the photonic signal from a light source such that power consumption is reduced or optimized. Parameters may include light intensity, firing rate, duty cycle, other suitable parameters, or any combination thereof. In some embodiments, the system may use information from a first light source to generate a light drive signal for a second light source. In some embodiments, the system may vary parameters in a way substantially synchronous with physiological pulses, for example, cardiac pulses. In some embodiments, the system may vary parameters in response to an external trigger.

32 Claims, 30 Drawing Sheets

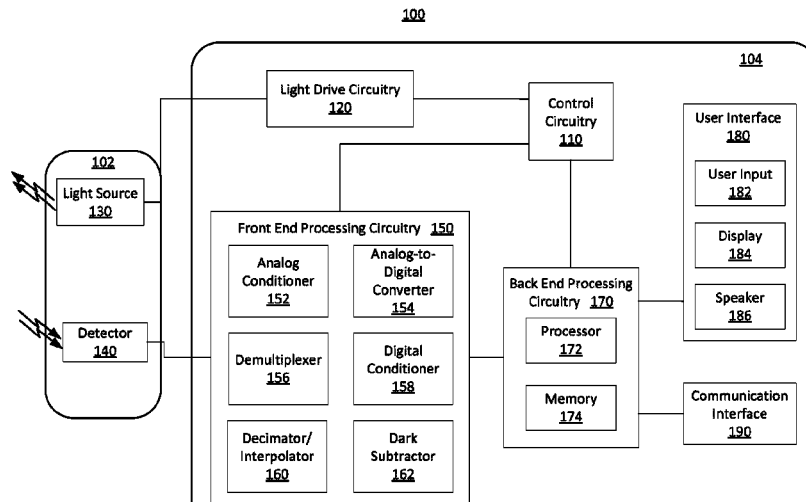

(56)

References Cited

U.S. PATENT DOCUMENTS

6,217,523 B1 4/2001 Amano et al.
6,226,539 B1 5/2001 Potratz
6,697,655 B2 2/2004 Sueppel et al.
6,697,658 B2 2/2004 Al-Ali
6,731,967 B1 5/2004 Turcott
6,863,652 B2 3/2005 Huang et al.
6,912,413 B2 6/2005 Rantala et al.
7,003,339 B2 2/2006 Diab et al.
7,120,479 B2 10/2006 Chew et al.
7,162,288 B2 1/2007 Nordstrom et al.
7,295,866 B2 11/2007 Al-Ali
7,382,247 B2 6/2008 Welch et al.

7,623,990 B2 11/2009 Anderson et al.
2005/0084202 A1 4/2005 Smith et al.
2005/0109339 A1 5/2005 Stahmann et al.
2006/0264720 A1 11/2006 Chew et al.
2007/0038049 A1 2/2007 Huang
2007/0149871 A1 6/2007 Sarussi et al.
2007/0208240 A1 9/2007 Nordstrom et al.
2011/0213397 A1 9/2011 Mathonnet
2011/0237911 A1 9/2011 Lamego et al.
2011/0245636 A1 10/2011 Li et al.

OTHER PUBLICATIONS

International Search Report and Written Opinion of the International Searching Authority for application No. PCT/US 2013/043338, mailed on Oct. 2, 2013.

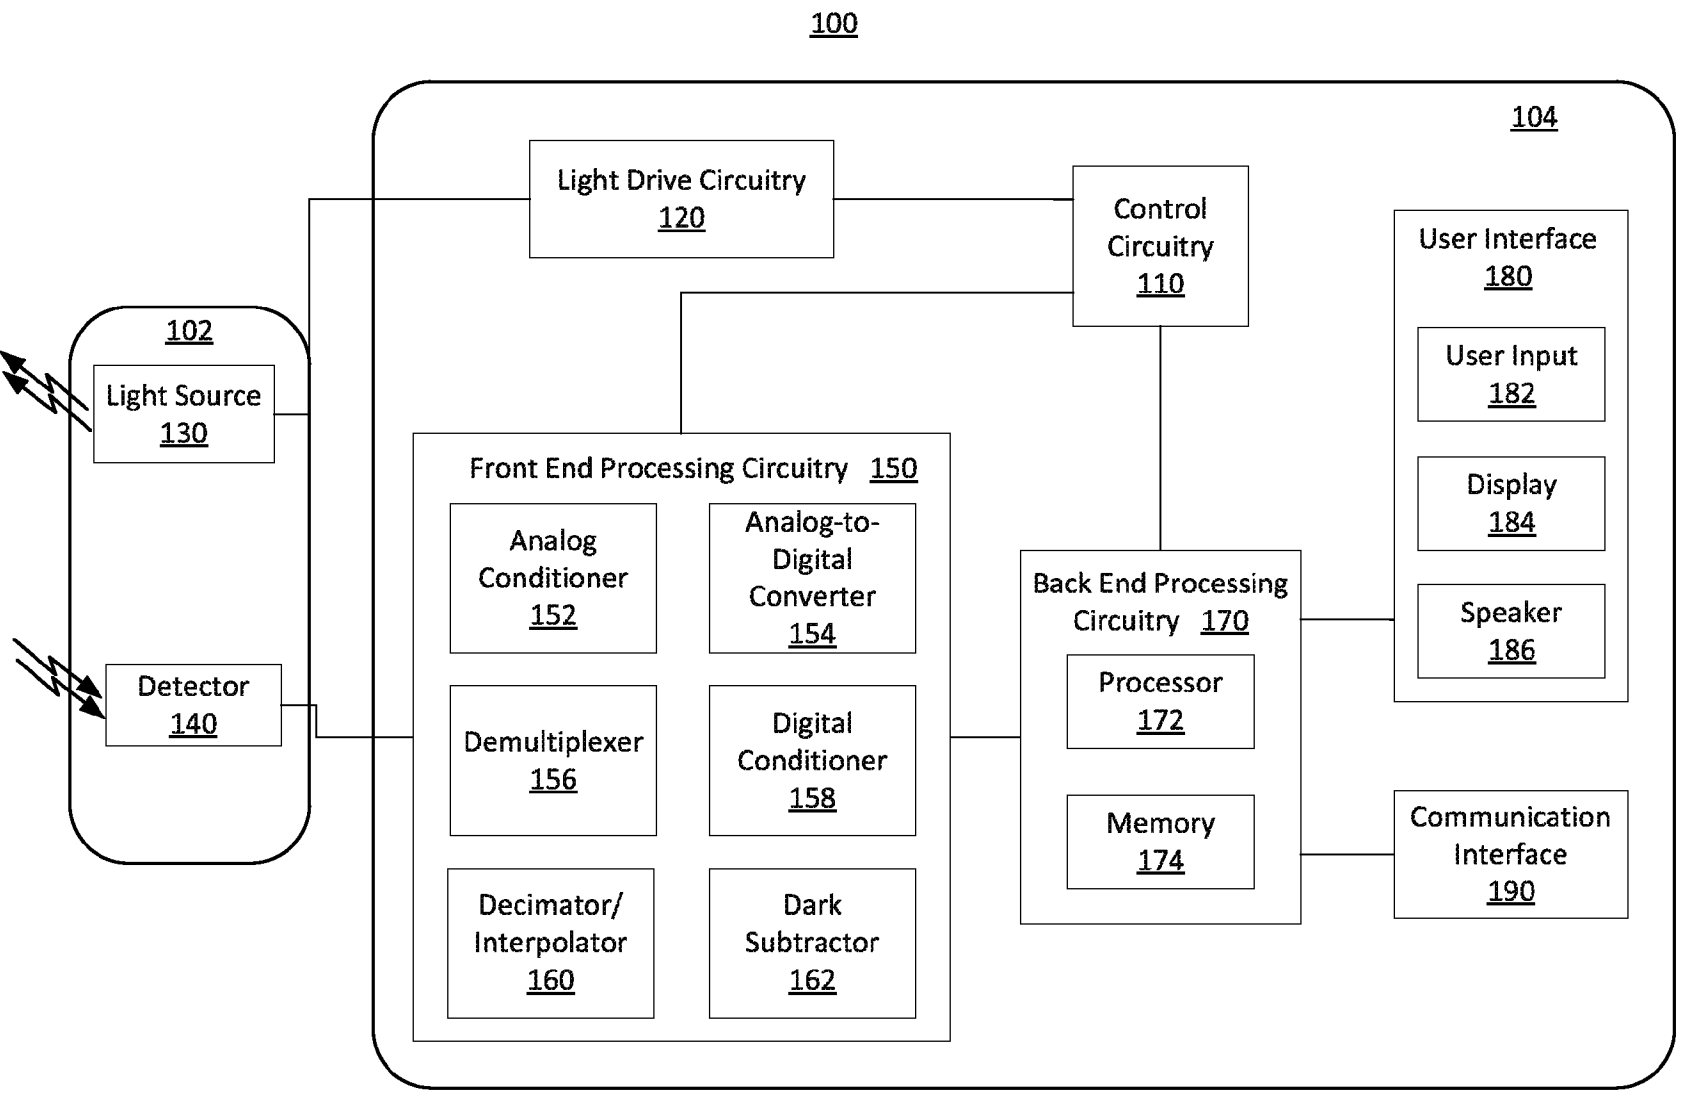


FIG. 1

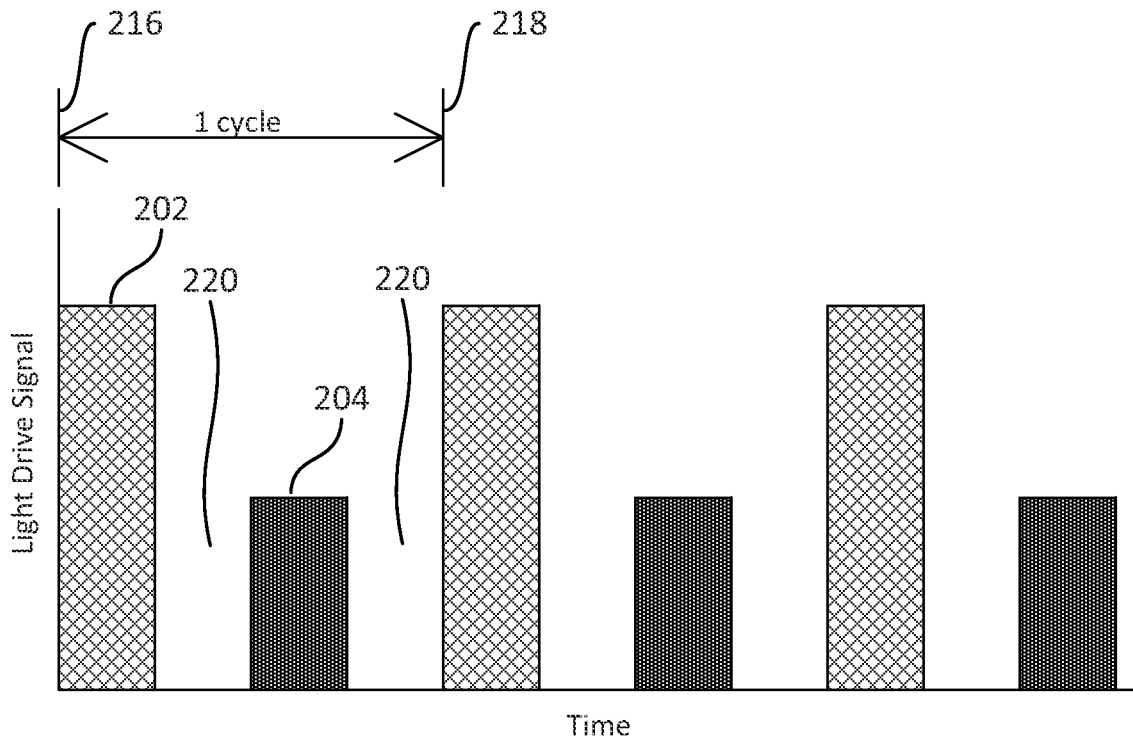


FIG. 2A

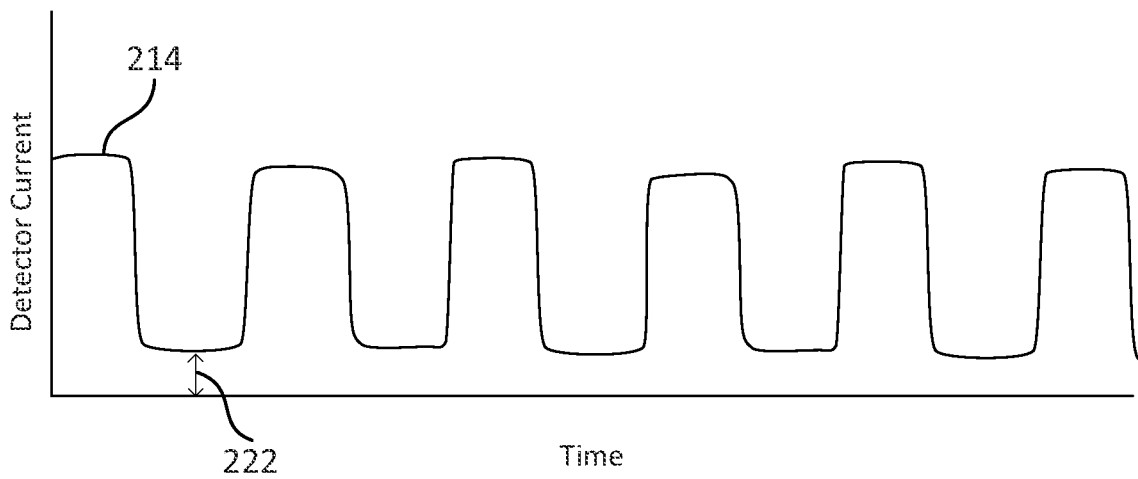


FIG. 2B

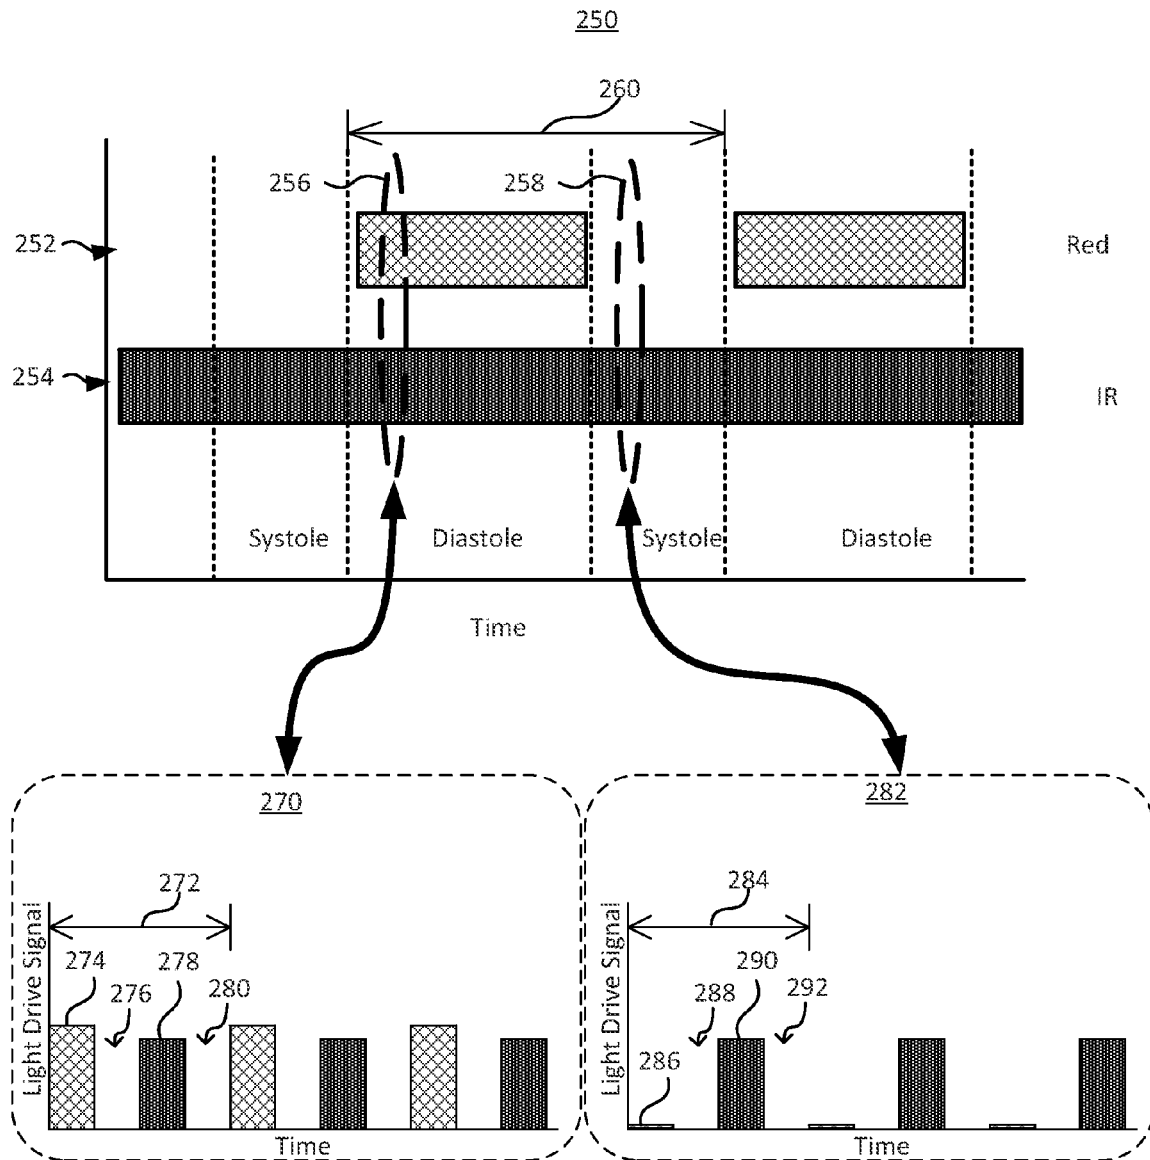


FIG. 2C

Explore Litigation Insights

Docket Alarm provides insights to develop a more informed litigation strategy and the peace of mind of knowing you're on top of things.

Real-Time Litigation Alerts



Keep your litigation team up-to-date with **real-time alerts** and advanced team management tools built for the enterprise, all while greatly reducing PACER spend.

Our comprehensive service means we can handle Federal, State, and Administrative courts across the country.

Advanced Docket Research



With over 230 million records, Docket Alarm's cloud-native docket research platform finds what other services can't. Coverage includes Federal, State, plus PTAB, TTAB, ITC and NLRB decisions, all in one place.

Identify arguments that have been successful in the past with full text, pinpoint searching. Link to case law cited within any court document via Fastcase.

Analytics At Your Fingertips



Learn what happened the last time a particular judge, opposing counsel or company faced cases similar to yours.

Advanced out-of-the-box PTAB and TTAB analytics are always at your fingertips.

API

Docket Alarm offers a powerful API (application programming interface) to developers that want to integrate case filings into their apps.

LAW FIRMS

Build custom dashboards for your attorneys and clients with live data direct from the court.

Automate many repetitive legal tasks like conflict checks, document management, and marketing.

FINANCIAL INSTITUTIONS

Litigation and bankruptcy checks for companies and debtors.

E-DISCOVERY AND LEGAL VENDORS

Sync your system to PACER to automate legal marketing.