

(12) **United States Patent**
Sigg et al.

(10) **Patent No.:** **US 9,220,631 B2**
(45) **Date of Patent:** **Dec. 29, 2015**

(54) **SYRINGE**

(71) Applicant: **Novartis AG**, Basel (CH)

(72) Inventors: **Juergen Sigg**, Loerrach (DE);
Christophe Royer, Munich (DE);
Andrew Mark Bryant, Basel Land (CH);
Heinrich Martin Buettgen, Rheinfelden (CH);
Marie Picci, Ranspack-le-bas (FR)

(73) Assignee: **Novartis AG**, Basel (CH)

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 0 days.

(21) Appl. No.: **13/750,352**

(22) Filed: **Jan. 25, 2013**

(65) **Prior Publication Data**

US 2014/0012227 A1 Jan. 9, 2014

(30) **Foreign Application Priority Data**

Jul. 30, 2012	(EP)	12174860
Oct. 23, 2012	(EP)	12189649
Nov. 16, 2012	(AU)	2012101677
Nov. 16, 2012	(AU)	2012101678
Nov. 16, 2012	(DE)	20 2012 011 016 U
Nov. 23, 2012	(DE)	20 2012 011 259 U
Nov. 23, 2012	(DE)	20 2012 011 260 U
Dec. 3, 2012	(EP)	12195360
Jan. 23, 2013	(AU)	2013100070
Jan. 23, 2013	(AU)	2013100071
Jan. 23, 2013	(DE)	20 2013 000 688 U

(51) **Int. Cl.**

A61M 5/00 (2006.01)
A61F 9/00 (2006.01)
A61M 5/178 (2006.01)

(Continued)

(52) **U.S. Cl.**

CPC **A61F 9/0008** (2013.01); **A61K 9/0019** (2013.01); **A61K 9/0048** (2013.01); **A61K 38/179** (2013.01); **A61M 5/002** (2013.01); **A61M 5/178** (2013.01); **A61M 5/28** (2013.01); **A61M 5/31** (2013.01); **A61M 5/315** (2013.01); **A61M 5/31505** (2013.01); **A61M 5/31513** (2013.01);

(Continued)

(58) **Field of Classification Search**

CPC **A61K 9/0048**; **A61F 9/0008**; **A61M 5/31**
USPC **604/218, 294**
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

6,090,081 A * 7/2000 Sudo et al. 604/230
7,141,042 B2 * 11/2006 Lubrecht 604/230

(Continued)

FOREIGN PATENT DOCUMENTS

AU 2012101677 A4 12/2012
AU 2012101678 A4 12/2012

(Continued)

OTHER PUBLICATIONS

Badkar et al., "Development of biotechnology products in pre-filled syringes: technical considerations and approaches", AAPS PharmaSciTech, vol. 12, No. 2, pp. 564-572, (Jun. 2011).

(Continued)


Primary Examiner — Aarti B Berdichevsky

(74) *Attorney, Agent, or Firm* — Michael Mazza

(57) **ABSTRACT**

The present invention relates to a syringe, particularly to a small volume syringe such as a syringe suitable for ophthalmic injections.

26 Claims, 1 Drawing Sheet

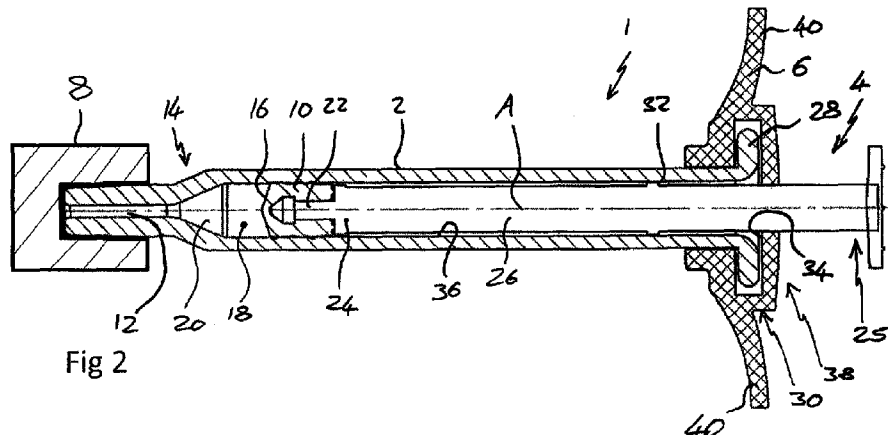

- (51) **Int. Cl.**
A61M 5/315 (2006.01)
A61K 9/00 (2006.01)
A61K 38/17 (2006.01)
A61M 5/28 (2006.01)
A61M 5/31 (2006.01)
- (52) **U.S. Cl.**
 CPC *A61M 2005/3104* (2013.01); *A61M 2005/3139* (2013.01)

(56) **References Cited**

U.S. PATENT DOCUMENTS

7,303,748	B2 *	12/2007	Wiegand et al.	424/134.1
2006/0172944	A1 *	8/2006	Wiegand et al.	514/12
2006/0293270	A1	12/2006	Adamis et al.	
2007/0190058	A1 *	8/2007	Shams	424/145.1
2008/0312607	A1 *	12/2008	Delmotte et al.	604/230
2010/0310309	A1	12/2010	Abendroth et al.	
2011/0257601	A1	10/2011	Furfine et al.	
2011/0276005	A1 *	11/2011	Hioki et al.	604/187
2012/0078224	A1	3/2012	Lerner et al.	
2013/0012918	A1	1/2013	Foster	
2014/0249484	A1 *	9/2014	Jones et al.	604/230

FOREIGN PATENT DOCUMENTS

CN	201578690	U	9/2010
DE	10 2008 005938	A1	7/2009
EP	0264273	A2	4/1988
EP	0879611	A2	11/1998
EP	2371406		10/2011
JP	2001-104480		4/2001
JP	2002241264	A2	8/2002
WO	97/44068	A1	11/1997
WO	2006047325	A1	5/2006
WO	2006128564	A1	12/2006
WO	WO 2007/035621	A1	3/2007
WO	2007084765	A2	7/2007
WO	WO 2007/149334	A2	12/2007
WO	WO2010/060748		6/2010
WO	2010136492		12/2010
WO	WO 2011/123722	A1	10/2011
WO	WO2011/135067		11/2011
WO	WO 2012/134528	A1	10/2012
WO	WO 2012/149040	A2	11/2012
WO	2014/005728	A1	1/2014

OTHER PUBLICATIONS

Ausubel et al., "Current Protocols in Molecular Biology", 7.7.18 of Current protocols in Molecular Biology, eds., supplement 30, (1987).
 Badkar et al., Analysis of Two Commercially Available Bortezomib Products : Differences in Assay of Active Agent and Impurity Profile >> AAPS PharmaSciTech, vol. 12, No. 2, pp. 564-572, (Jun. 2011).

Schoenknecht, "Requirements on pre-fillable glass syringes", AAPS National Biotechnology Conference 2007—Abstract No. NBC07-000488, 2007.
 Holash et al., "VEGF-Trap: A VEGF blocker with potent anitumor effects", PNAS USA, vol. 99, No. 17, pp. 11393-11398, (Aug. 20, 2002).
 Riely & Miller, "Vascular Endothelial Growth Factor Trap in Non-Small Cell lung Cancer", Clin Cancer Res, 13:4623-7s, (Aug. 1, 2007).
 Li et al., "KH906, a recombinant human VEGF receptor fusion protein, is a new effective topical treatment for corneal neovascularization", Molecular Vision, 17:797-803,(Mar. 25, 2011).
 Smith & Waterman, "Comparison of Biosequences", Adv Appl. Math, 2:482-489, (1981).
 Chan et al: "Syringe Siliconization Process Investigation and Optimization" Journal of Pharmaceutical Science and Technology, Issue 66, pp. 137, 147-148, Mar. 2012.
 Lankers: "The Relationship Between Silicone Layer Thickness, Free Silicone Oil and Protein Aggregation in Prefilled Syringes" 2010 AAPS National Biotechnology Conference San Francisco, Slides 25, 39, 46, May 19, 2010.
 Majumdar et al: "Evaluation of the Effect of Syringe Surfaces on Protein Formulations" Journal of Pharmaceutical Sciences, Issue 100, pp. 2563-2573, Jul. 2011.
 Bakri and Ekdawi: "Intravitreal Silicone Oil Droplets after Intravitreal Drug Injections" Retina, Issue 28, pp. 996-1001, Jul. 2008.
 Daikyo Ru Crystal Zenith Insert Needle Syringe System, West Delivering Innovative Solutions, 2010.
 Meyer et al: "Steps for a Safe Intravitreal Injection Technique",Meyer et al. "Steps for a Safe Intravitreal Injection Technique"Retinal Physician, p. 3, Jul. 1, 2009.
 "Biopharmaceuticals—SPE applications", RapID Particle Systems, Single Particle Explore, D6a, Sep. 28, 2015, <http://www.particle-explorer.com/yourapplications/biopharmaceuticals/index.html>[Sep. 16, 2015 11:12:45].
 Email dated Sep. 9, 2015 from Elizabeth Scuderl, Senior meeting Manager, AAPS to Teresa Homnch re Inquiry about publication of conference abstract.
 Tibor Hlobik: "Reducing quality risks to drug products and meeting needs of patients with enhanced components for prefilled syringe systems". West Delivering Innovative Solutions, www.ondrugdelivery.com, 2012 No. 33, pp. 32-34.
 Summary of Product Characteristics—Zaltrap (undated).
 "Ranibizumab", Scientific Discussion, EMEA, 2007, pp. 1-54.
 "Avastin", Scientific Discussion, EMEA, 2005, pp. 1-61.
 Melmet Selim Kocabora, et al. "Intreavitreal silicone oil droplets following pegaptanib injection", Acta Ophthalmologica, 2010 e44-345.
 N. Clunas, et al: "Ranibizumab pre-filled syringe: recently approved innovation in the European Union with the potential to reduce infection risk, improve does accuracy, and enhance efficient treatment administration". Congress on Controversies in Ophthalmology, Abstract, 2014.
 "COPHy Poster List—Group A"(Poster 17), The 5th World congress on Controversies in Ophthalmology (COPHy) Mar. 20-23, 2014, Lisbon, Portugal.

* cited by examiner

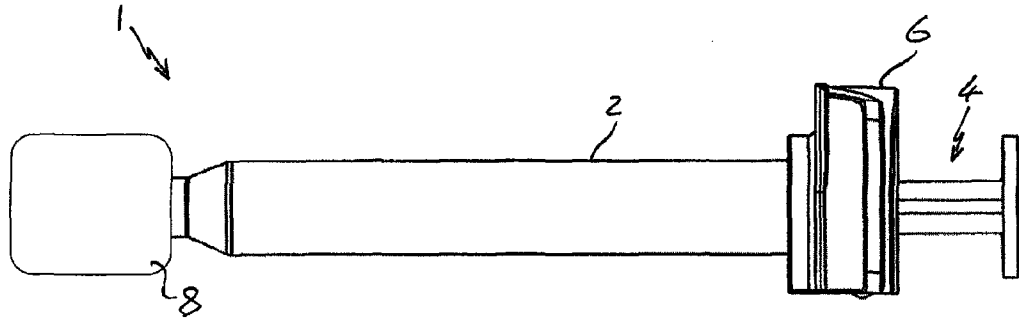


Fig 1

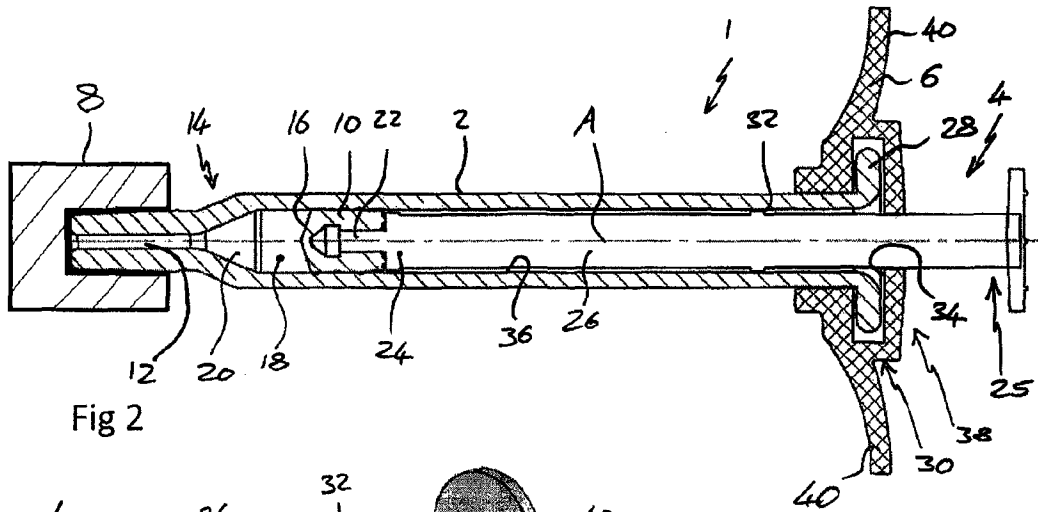


Fig 2

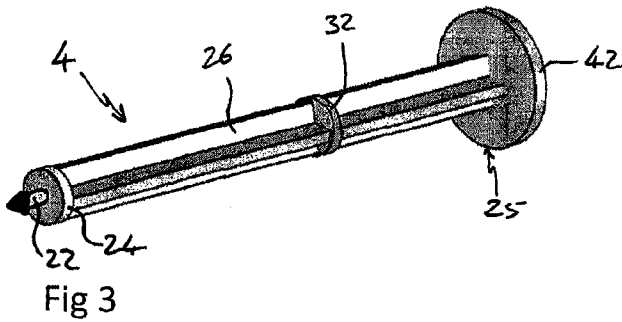


Fig 3

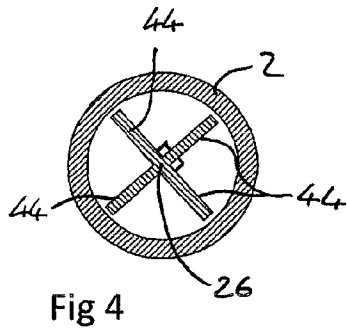


Fig 4

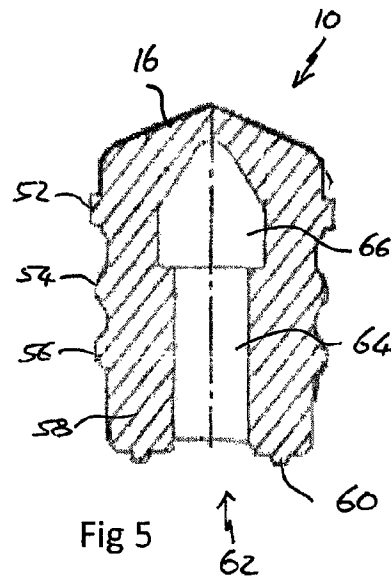


Fig 5

TECHNICAL FIELD

The present invention relates to a syringe, particularly to a small volume syringe such as a syringe suitable for ophthalmic injections.

BACKGROUND ART

Many medicaments are delivered to a patient in a syringe from which the user can dispense the medicament. If medicament is delivered to a patient in a syringe it is often to enable the patient, or a caregiver, to inject the medicament. It is important for patient safety and medicament integrity that the syringe and the contents of that syringe are sufficiently sterile to avoid infection, or other, risks for patients. Sterilisation can be achieved by terminal sterilisation in which the assembled product, typically already in its associated packaging, is sterilised using heat or a sterilising gas.

For small volume syringes, for example those for injections into the eye in which it is intended that about 0.1 ml or less of liquid is to be injected the sterilisation can pose difficulties that are not necessarily associated with larger syringes. Changes in pressure, internal or external to the syringe, can cause parts of the syringe to move unpredictably, which may alter sealing characteristics and potentially compromise sterility. Incorrect handling of the syringe can also pose risks to product sterility.

Furthermore, certain therapeutics such as biologic molecules are particularly sensitive to sterilisation, be it cold gas sterilisation, thermal sterilisation, or irradiation. Thus, a careful balancing act is required to ensure that while a suitable level of sterilisation is carried out, the syringe remains suitably sealed, such that the therapeutic is not compromised. Of course, the syringe must also remain easy to use, in that the force required to depress the plunger to administer the medicament must not be too high.

There is therefore a need for a new syringe construct which provides a robust seal for its content, but which maintains ease of use.

DISCLOSURE OF THE INVENTION

The present invention provides a pre-filled syringe, the syringe comprising a body, a stopper and a plunger, the body comprising an outlet at an outlet end and the stopper being arranged within the body such that a front surface of the stopper and the body define a variable volume chamber from which a fluid can be expelled through the outlet, the plunger comprising a plunger contact surface at a first end and a rod extending between the plunger contact surface and a rear portion, the plunger contact surface arranged to contact the stopper, such that the plunger can be used to force the stopper towards the outlet end of the body, reducing the volume of the variable volume chamber, characterised in that the fluid comprises an ophthalmic solution. In one embodiment, the ophthalmic solution comprises a VEGF-antagonist.

In one embodiment, the syringe is suitable for ophthalmic injections, more particularly intravitreal injections, and as such has a suitably small volume. The syringe may also be silicone oil free, or substantially silicone oil free, or may comprise a low level of silicone oil as lubricant. In one embodiment, despite the low silicone oil level, the stopper break loose and slide force is less than 20N.

For ophthalmic injections, it is particularly important for the ophthalmic solution to have particularly low particle content. In one embodiment, the syringe meets US Pharmacopeia standard 789 (USP789).

Syringe

The body of the syringe may be a substantially cylindrical shell, or may include a substantially cylindrical bore with a non circular outer shape. The outlet end of the body includes an outlet through which a fluid housed within the variable volume chamber can be expelled as the volume of said chamber is reduced. The outlet may comprise a projection from the outlet end through which extends a channel having a smaller diameter than that of the variable volume chamber. The outlet may be adapted, for example via a luer lock type connection, for connection to a needle or other accessory such as a sealing device which is able to seal the variable volume chamber, but can be operated, or removed, to unseal the variable volume chamber and allow connection of the syringe to another accessory, such as a needle. Such a connection may be made directly between the syringe and accessory, or via the sealing device. The body extends along a first axis from the outlet end to a rear end.

The body may be made from a plastic material (e.g. a cyclic olefin polymer) or from glass and may include indicia on a surface thereof to act as an injection guide. In one embodiment the body may comprise a priming mark. This allows the physician to align a pre-determined part of the stopper (such as the tip of the front surface or one of the circumferential ribs, discussed later) or plunger with the mark, thus expelling excess ophthalmic solution and any air bubbles from the syringe. The priming process ensures that an exact, pre-determined dosage is administered to the patient.

The stopper may be made from rubber, silicone or other suitable resiliently deformable material. The stopper may be substantially cylindrical and the stopper may include one or more circumferential ribs around an outer surface of the stopper, the stopper and ribs being dimensioned such that the ribs form a substantially fluid tight seal with an internal surface of the syringe body. The front surface of the stopper may be any suitable shape, for example substantially planar, substantially conical or of a domed shape. The rear surface of the stopper may include a substantially central recess. Such a central recess could be used to connect a plunger to the stopper using a snap fit feature or thread connection in a known manner. The stopper may be substantially rotationally symmetric about an axis through the stopper.

The plunger comprises a plunger contact surface and extending from that a rod extends from the plunger contact surface to a rear portion. The rear portion may include a user contact portion adapted to be contacted by a user during an injection event. The user contact portion may comprise a substantially disc shaped portion, the radius of the disc extending substantially perpendicular to the axis along which the rod extends. The user contact portion could be any suitable shape. The axis along which the rod extends may be the first axis, or may be substantially parallel with the first axis.

The syringe may include a backstop arranged at a rear portion of the body. The backstop may be removable from the syringe. If the syringe body includes terminal flanges at the end opposite the outlet end the backstop may be configured to substantially sandwich terminal flanges of the body as this prevent movement of the backstop in a direction parallel to the first axis.

The rod may comprise at least one rod shoulder directed away from the outlet end and the backstop may include a backstop shoulder directed towards the outlet end to cooperate with the rod shoulder to substantially prevent movement

of the rod away from the outlet end when the backstop shoulder and rod shoulder are in contact. Restriction of the movement of the rod away from the outlet end can help to maintain sterility during terminal sterilisation operations, or other operations in which the pressure within the variable volume chamber or outside the chamber may change. During such operations any gas trapped within the variable volume chamber, or bubbles that may form in a liquid therein, may change in volume and thereby cause the stopper to move. Movement of the stopper away from the outlet could result in the breaching of a sterility zone created by the stopper. This is particularly important for low volume syringes where there are much lower tolerances in the component sizes and less flexibility in the stopper. The term sterility zone as used herein is used to refer to the area within the syringe that is sealed by the stopper from access from either end of the syringe. This may be the area between a seal of the stopper, for example a circumferential rib, closest to the outlet and a seal of the stopper, for example a circumferential rib, furthest from the outlet. The distance between these two seals defines the sterility zone of the stopper since the stopper is installed into the syringe barrel in a sterile environment.

To further assist in maintaining sterility during the operations noted above the stopper may comprise at a front circumferential rib and a rear circumferential rib and those ribs may be separated in a direction along the first axis by at least 3 mm, by at least 3.5 mm, by at least 3.75 mm or by 4 mm or more. One or more additional ribs (for example 2, 3, 4 or 5 additional ribs, or between 1-10, 2-8, 3-6 or 4-5 additional ribs) may be arranged between the front and rear ribs. In one embodiment there are a total of three circumferential ribs.

A stopper with such an enhanced sterility zone can also provide protection for the injectable medicament during a terminal sterilisation process. More ribs on the stopper, or a greater distance between the front and rear ribs can reduce the potential exposure of the medicament to the sterilising agent. However, increasing the number of ribs can increase the friction between the stopper and syringe body, reducing ease of use. While this may be overcome by increasing the silicisation of the syringe, such an increase in silicone oil levels is particularly undesirable for syringes for ophthalmic use.

The rod shoulder may be arranged within the external diameter of the rod, or may be arranged outside the external diameter of the rod. By providing a shoulder that extends beyond the external diameter of the rod, but still fits within the body, the shoulder can help to stabilise the movement of the rod within the body by reducing movement of the rod perpendicular to the first axis. The rod shoulder may comprise any suitable shoulder forming elements on the rod, but in one embodiment the rod shoulder comprises a substantially disc shaped portion on the rod.

In one embodiment of the syringe, when arranged with the plunger contact surface in contact with the stopper and the variable volume chamber is at its intended maximum volume there is a clearance of no more than about 2 mm between the rod shoulder and backstop shoulder. In some embodiments there is a clearance of less than about 1.5 mm and in some less than about 1 mm. This distance is selected to substantially limit or prevent excessive rearward (away from the outlet end) movement of the stopper.

In one embodiment the variable volume chamber has an internal diameter greater than 5 mm or 6 mm, or less than 3 mm or 4 mm. The internal diameter may be between 3 mm and 6 mm, or between 4 mm and 5 mm.

In another embodiment the syringe is dimensioned so as to have a nominal maximum fill volume of between about 0.1 ml

and about 1.5 ml. In certain embodiments the nominal maximum fill volume is between about 0.5 ml and about 1 ml. In certain embodiments the nominal maximum fill volume is about 0.5 ml or about 1 ml, or about 1.5 ml.

The length of the body of the syringe may be less than 70 mm, less than 60 mm or less than 50 mm. In one embodiment the length of the syringe body is between 45 mm and 50 mm.

In one embodiment, the syringe is filled with between about 0.01 ml and about 1.5 ml (for example between about 0.05 ml and about 1 ml, between about 0.1 ml and about 0.5 ml, between about 0.15 ml and about 0.175 ml) of a VEGF antagonist solution. In one embodiment, the syringe is filled with 0.165 ml of a VEGF antagonist solution. Of course, typically a syringe is filled with more than the desired dose to be administered to the patient, to take into account wastage due to "dead space" within the syringe and needle. There may also be a certain amount of wastage when the syringe is primed by the physician, so that it is ready to inject the patient.

Thus, in one embodiment, the syringe is filled with a dosage volume (i.e. the volume of medicament intended for delivery to the patient) of between about 0.01 ml and about 1.5 ml (e.g. between about 0.05 ml and about 1 ml, between about 0.1 ml and about 0.5 ml) of a VEGF antagonist solution. In one embodiment, the dosage volume is between about 0.03 ml and about 0.05 ml. For example, for Lucentis, the dosage volume is 0.05 ml or 0.03 ml (0.5 mg or 0.3 mg) of a 10 mg/ml injectable medicament solution; for Eylea, the dosage volume is 0.05 ml of a 40 mg/ml injectable medicament solution. Although unapproved for ophthalmic indications, bevacizumab is used off-label in such ophthalmic indications at a concentration of 25 mg/ml; typically at a dosage volume of 0.05 ml (1.25 mg). In one embodiment, the extractable volume from the syringe (that is the amount of product obtainable from the syringe following filling, taking into account loss due to dead space in the syringe and needle) is about 0.09 ml.

In one embodiment the length of the syringe body is between about 45 mm and about 50 mm, the internal diameter is between about 4 mm and about 5 mm, the fill volume is between about 0.12 and about 0.3 ml and the dosage volume is between about 0.03 ml and about 0.05 ml.

As the syringe contains a medicament solution, the outlet may be reversibly sealed to maintain sterility of the medicament. This sealing may be achieved through the use of a sealing device as is known in the art. For example the OVS™ system which is available from Vetter Pharma International GmbH.

It is typical to silicise the syringe in order to allow ease of use, i.e. to apply silicone oil to the inside of the barrel, which decreases the force required to move the stopper. However, for ophthalmic use, it is desirable to decrease the likelihood of silicone oil droplets being injected into the eye. With multiple injections, the amount of silicone droplets can build up in the eye, causing potential adverse effects, including "floaters" and an increase in intra-ocular pressure. Furthermore, silicone oil can cause proteins to aggregate. A typical 1 ml syringe comprises 100-800 µg silicone oil in the barrel, though a survey of manufacturers reported that 500-1000 µg was typically used in pre-filled syringes (Badkar et al. 2011, AAPS PharmaSciTech, 12(2):564-572). Thus, in one embodiment, a syringe according to the invention comprises less than about 800 µg (i.e. about less than about 500 µg, less than about 300 µg, less than about 200 µg, less than about 100 µg, less than about 75 µg, less than about 50 µg, less than about 25 µg, less than about 15 µg, less than about 10 µg) silicone oil in the barrel. If the syringe comprises a low level of silicone oil, this may be more than about 1 µg, more than

Explore Litigation Insights

Docket Alarm provides insights to develop a more informed litigation strategy and the peace of mind of knowing you're on top of things.

Real-Time Litigation Alerts



Keep your litigation team up-to-date with **real-time alerts** and advanced team management tools built for the enterprise, all while greatly reducing PACER spend.

Our comprehensive service means we can handle Federal, State, and Administrative courts across the country.

Advanced Docket Research



With over 230 million records, Docket Alarm's cloud-native docket research platform finds what other services can't. Coverage includes Federal, State, plus PTAB, TTAB, ITC and NLRB decisions, all in one place.

Identify arguments that have been successful in the past with full text, pinpoint searching. Link to case law cited within any court document via Fastcase.

Analytics At Your Fingertips



Learn what happened the last time a particular judge, opposing counsel or company faced cases similar to yours.

Advanced out-of-the-box PTAB and TTAB analytics are always at your fingertips.

API

Docket Alarm offers a powerful API (application programming interface) to developers that want to integrate case filings into their apps.

LAW FIRMS

Build custom dashboards for your attorneys and clients with live data direct from the court.

Automate many repetitive legal tasks like conflict checks, document management, and marketing.

FINANCIAL INSTITUTIONS

Litigation and bankruptcy checks for companies and debtors.

E-DISCOVERY AND LEGAL VENDORS

Sync your system to PACER to automate legal marketing.