



US005176137A

United States Patent [19]

[11] Patent Number: 5,176,137

Erickson et al.

[45] Date of Patent: Jan. 5, 1993

- [54] APPARATUS FOR DISCRIMINATION OF STABLE AND UNSTABLE VENTRICULAR TACHYCARDIA AND FOR TREATMENT THEREOF
- [75] Inventors: Mark K. Erickson, Minneapolis; Tom D. Bennett, Shoreview, both of Minn.
- [73] Assignee: Medtronic, Inc., Minneapolis, Minn.
- [21] Appl. No.: 663,985
- [22] Filed: Mar. 1, 1991
- [51] Int. Cl.⁵ A61N 1/39
- [52] U.S. Cl. 128/419 D
- [58] Field of Search 128/419 D, 419 PG

matic and Completely Implanted System”, Transactions American Society for Artificial Internal Organs, 16:207 1970, by Schuder et al.
 “Automatic Implantable Cardioverter-Defibrillator Structural Characteristics”, PACE, vol. 7, Nov.-Dec. 1984, Part II, pp. 1331-1334, by Mower et al.
 “Reliable R-Wave Detection from Ambulatory Subjects”, by Thakor, Biomed Sci Instrum 14:67-72, 1978.
 “Relationship Between Right Atrial and Mixed Venous Oxygen Saturation and Heart Rate During Exercise in Normal Subjects and Patients with Cardiac Disease” by a French et al.

Primary Examiner—William E. Kamm
 Attorney, Agent, or Firm—Reed A. Duthler; Harold R. Patton

[56] References Cited

U.S. PATENT DOCUMENTS

- Re. 27,757 3/1987 Mirowski .
- 3,737,579 6/1973 Bolduc .
- 4,114,628 9/1978 Rizk .
- 4,240,442 12/1980 Andresen et al. .
- 4,291,699 9/1981 Geddes et al. .
- 4,375,817 3/1983 Engle et al. .
- 4,384,585 5/1983 Zipes .
- 4,523,595 6/1985 Zibell .
- 4,548,209 10/1985 Wielders et al. .
- 4,577,633 3/1986 Berkovits et al. .
- 4,587,970 5/1986 Holley et al. .
- 4,693,253 9/1987 Adams .
- 4,726,380 2/1988 Vollmann et al. .
- 4,750,495 6/1988 Moore et al. .
- 4,774,950 10/1988 Cohen .
- 4,800,883 1/1989 Winstrom .
- 4,817,634 4/1989 Holleman et al. .
- 4,819,643 4/1989 Menken .
- 4,830,006 5/1989 Haluska et al. .
- 4,880,004 11/1989 Baker, Jr. et al. .
- 4,880,005 11/1989 Pless et al. .
- 4,949,719 8/1990 Pless et al. .
- 4,953,551 9/1990 Mehra et al. .
- 4,967,748 11/1990 Cohen .
- 4,967,749 11/1990 Cohen .


[57] ABSTRACT

A method and apparatus for discriminating between stable and unstable ventricular tachycardias based on a measurement of oxygen saturation. Reference values for average oxygen saturation level and of the pulsatile characteristic of the oxygen saturation level are taken while a patient is in a resting condition. Measurements of oxygen saturation are also taken in response to the detection of a high heart rate, and are compared to the reference measurements to discriminate between stable and unstable ventricular tachyarrhythmias. An unstable tachyarrhythmia is diagnosed if a tachycardia is diagnosed and the current oxygen saturation level is similar to the reference average oxygen saturation level or if the oxygen saturation as presently measured displays a decreased pulsatile characteristic as compared to the reference measurements. The discriminator is intended for use in conjunction with or as part of an automated cardioverter of the type capable of delivering differing therapies for termination of stable and unstable ventricular tachyarrhythmias, such as antitachycardia pacing, cardioversion and defibrillation.

OTHER PUBLICATIONS

“Experimental Ventricular Defibrillation with an Auto-

20 Claims, 7 Drawing Sheets

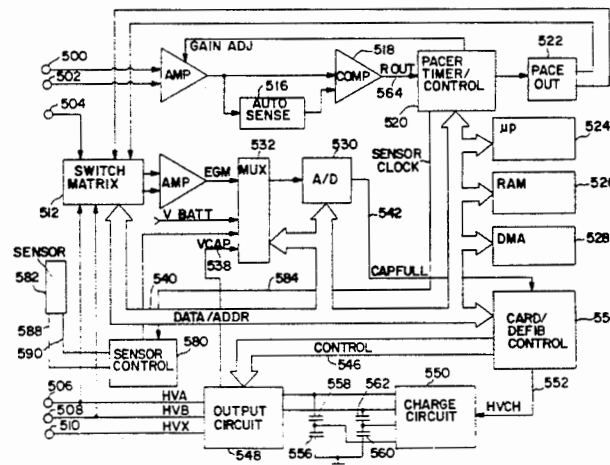

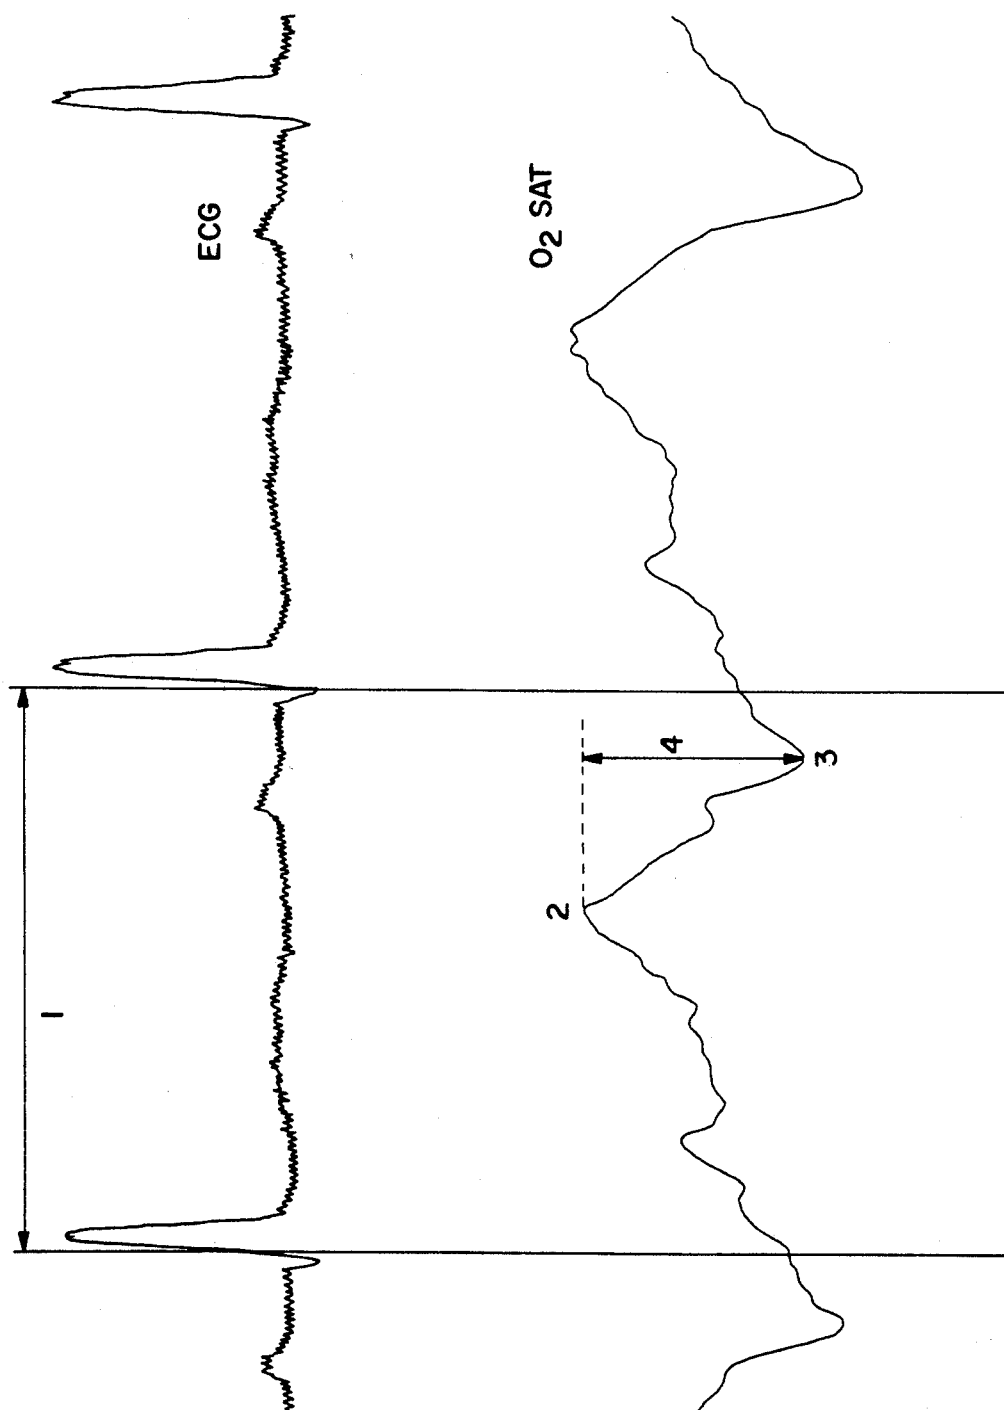


FIG. 1

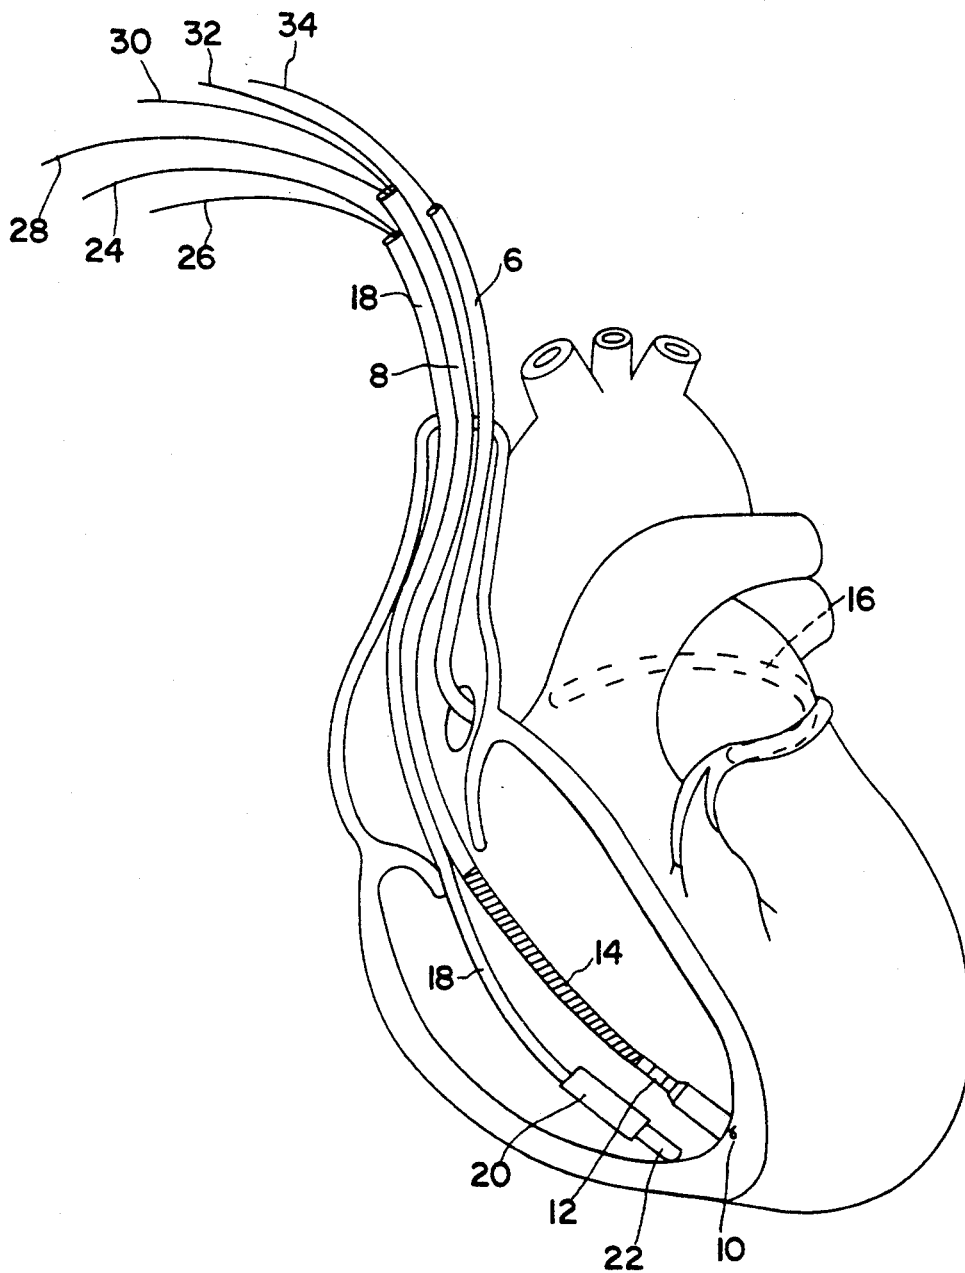


FIG.2

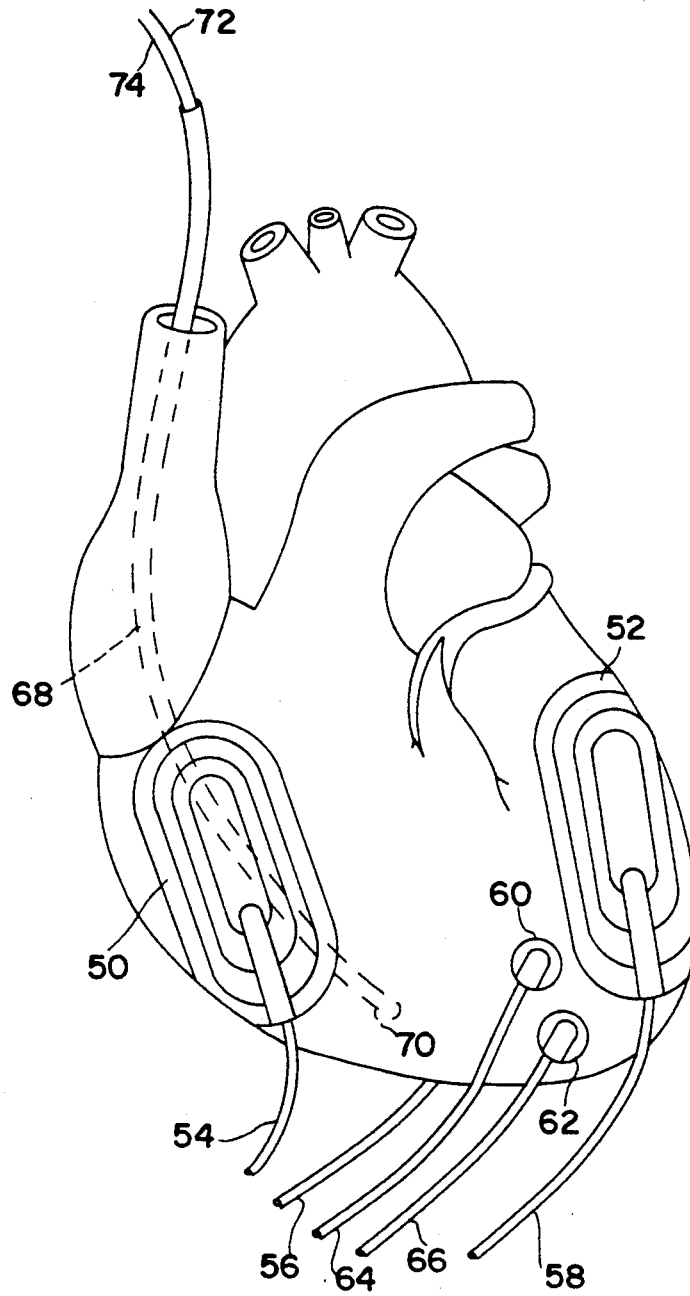


FIG. 3

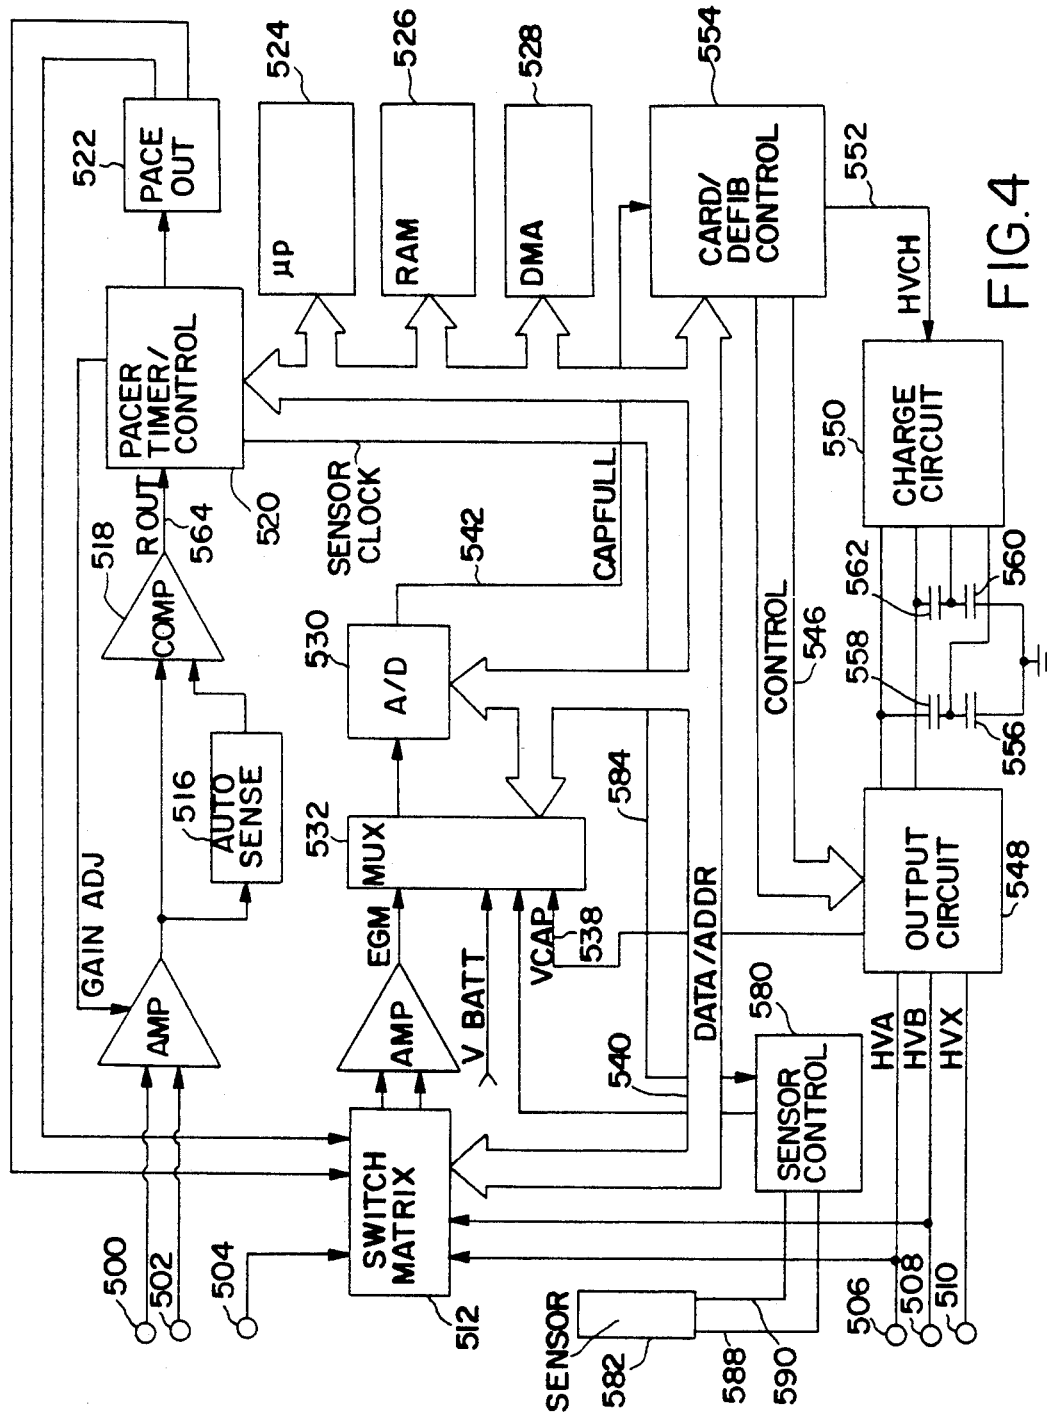


FIG. 4

Explore Litigation Insights

Docket Alarm provides insights to develop a more informed litigation strategy and the peace of mind of knowing you're on top of things.

Real-Time Litigation Alerts



Keep your litigation team up-to-date with **real-time alerts** and advanced team management tools built for the enterprise, all while greatly reducing PACER spend.

Our comprehensive service means we can handle Federal, State, and Administrative courts across the country.

Advanced Docket Research



With over 230 million records, Docket Alarm's cloud-native docket research platform finds what other services can't. Coverage includes Federal, State, plus PTAB, TTAB, ITC and NLRB decisions, all in one place.

Identify arguments that have been successful in the past with full text, pinpoint searching. Link to case law cited within any court document via Fastcase.

Analytics At Your Fingertips



Learn what happened the last time a particular judge, opposing counsel or company faced cases similar to yours.

Advanced out-of-the-box PTAB and TTAB analytics are always at your fingertips.

API

Docket Alarm offers a powerful API (application programming interface) to developers that want to integrate case filings into their apps.

LAW FIRMS

Build custom dashboards for your attorneys and clients with live data direct from the court.

Automate many repetitive legal tasks like conflict checks, document management, and marketing.

FINANCIAL INSTITUTIONS

Litigation and bankruptcy checks for companies and debtors.

E-DISCOVERY AND LEGAL VENDORS

Sync your system to PACER to automate legal marketing.