



US008942387B2

(12) **United States Patent**
Elko et al.

(10) **Patent No.:** **US 8,942,387 B2**
(45) **Date of Patent:** **Jan. 27, 2015**

(54) **NOISE-REDUCING DIRECTIONAL MICROPHONE ARRAY**

2410/07 (2013.01); H04R 2430/20 (2013.01);
H04R 2430/21 (2013.01); H04R 2430/23
(2013.01)

(75) Inventors: **Gary W. Elko**, Summit, NJ (US); **Jens M. Meyer**, Fairfax, VT (US); **Tomas Fritz Gaensler**, Warren, NJ (US)

USPC **381/94.2**; 381/94.1; 381/92
(58) **Field of Classification Search**
USPC 381/94.1, 94.2, 92.3, 92, 56
See application file for complete search history.

(73) Assignee: **MH Acoustics LLC**, Summit, NJ (US)

(56) **References Cited**

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 1194 days.

U.S. PATENT DOCUMENTS

3,626,365 A 12/1971 Press
4,281,551 A * 8/1981 Gaudriot et al. 73/647
(Continued)

(21) Appl. No.: **12/281,447**

FOREIGN PATENT DOCUMENTS

(22) PCT Filed: **Mar. 9, 2007**

EP 1 581 026 A1 9/2005
JP H06-269084 A 9/1994

(86) PCT No.: **PCT/US2007/006093**

§ 371 (c)(1),
(2), (4) Date: **Sep. 2, 2008**

(Continued)

OTHER PUBLICATIONS

(87) PCT Pub. No.: **WO2007/106399**

PCT Pub. Date: **Sep. 20, 2007**

Olson, HF (1946), Gradient Microphones. Journal of the Acoustic Society of America, vol. 17, No. 3, pp. 192-198.*

(Continued)

(65) **Prior Publication Data**

US 2009/0175466 A1 Jul. 9, 2009

Primary Examiner — Duc Nguyen

Assistant Examiner — Kile Blair

(74) *Attorney, Agent, or Firm* — Mendelsohn, Drucker & Dunleavy, P.C.; Steve Mendelsohn

Related U.S. Application Data

(63) Continuation-in-part of application No. PCT/US2006/044427, filed on Nov. 15, 2006, and a continuation-in-part of application No. 10/193,825, filed on Jul. 12, 2002, now Pat. No. 7,171,008.

(Continued)

(57) **ABSTRACT**


In one embodiment, a directional microphone array having (at least) two microphones generates forward and backward cardioid signals from two (e.g., omnidirectional) microphone signals. An adaptation factor is applied to the backward cardioid signal, and the resulting adjusted backward cardioid signal is subtracted from the forward cardioid signal to generate a (first-order) output audio signal corresponding to a beampattern having no nulls for negative values of the adaptation factor. After low-pass filtering, spatial noise suppression can be applied to the output audio signal. Microphone arrays having one (or more) additional microphones can be designed to generate second- (or higher-) order output audio signals.

(51) **Int. Cl.**
H04B 15/00 (2006.01)
H04R 3/00 (2006.01)

(Continued)

(52) **U.S. Cl.**
CPC **H04R 3/005** (2013.01); **H04R 25/407** (2013.01); **G10L 2021/02166** (2013.01); **H04R**

55 Claims, 15 Drawing Sheets

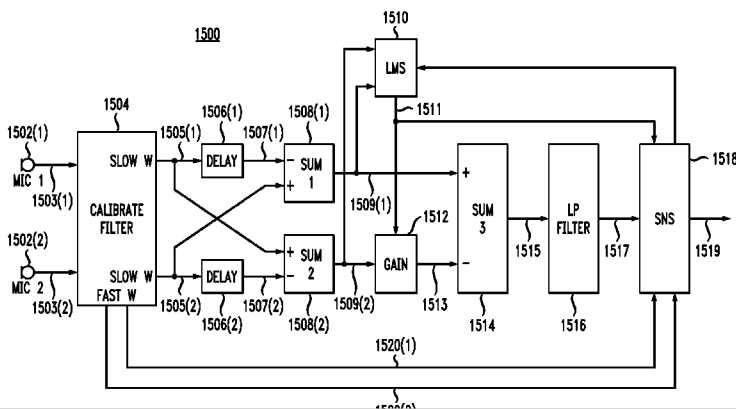

Related U.S. Application Data

(60) Provisional application No. 60/781,250, filed on Mar. 10, 2006, provisional application No. 60/737,577, filed on Nov. 17, 2005, provisional application No. 60/354,650, filed on Feb. 5, 2002.

(51) **Int. Cl.**
H04R 25/00 (2006.01)
G10L 21/0216 (2013.01)

References Cited

U.S. PATENT DOCUMENTS

4,741,038 A 4/1988 Elko et al.
 5,325,872 A 7/1994 Westermann
 5,473,701 A * 12/1995 Cezanne et al.
 5,515,445 A 5/1996 Baumhauer, Jr. et al.
 5,524,056 A 6/1996 Killion et al.
 5,602,962 A 2/1997 Kellermann
 5,610,991 A 3/1997 Janse
 5,687,241 A 11/1997 Ludvigsen
 5,878,146 A 3/1999 Andersen
 5,982,906 A * 11/1999 Ono 381/94.2
 6,041,127 A * 3/2000 Elko 381/92
 6,272,229 B1 8/2001 Baekgaard
 6,292,571 B1 9/2001 Sjursen
 6,339,647 B1 1/2002 Andersen et al.
 6,584,203 B2 * 6/2003 Elko et al.
 6,668,062 B1 * 12/2003 Luo et al.
 6,983,055 B2 1/2006 Luo
 7,242,781 B2 * 7/2007 Hou
 7,577,262 B2 * 8/2009 Kanamori et al.
 7,817,808 B2 * 10/2010 Konchitsky et al.
 8,135,142 B2 3/2012 Fischer et al.
 2003/0031328 A1 * 2/2003 Elko et al. 381/92
 2003/0053646 A1 3/2003 Nielsen et al.
 2003/0147538 A1 8/2003 Elko 381/92
 2003/0206640 A1 * 11/2003 Malvar et al. 381/93
 2004/0022397 A1 * 2/2004 Warren 381/92
 2004/0165736 A1 * 8/2004 Hetherington et al. 381/94.3
 2005/0276423 A1 12/2005 Aubauer et al.
 2006/0115103 A1 * 6/2006 Feng et al. 381/313
 2009/0175466 A1 * 7/2009 Elko et al. 381/94.2
 2009/0323982 A1 * 12/2009 Solbach et al. 381/94.3
 2010/0329492 A1 * 12/2010 Derleth et al. 381/317

FOREIGN PATENT DOCUMENTS

JP 06-303689 10/1994
 JP 10023590 A * 1/1998
 JP 10126878 A * 5/1998
 JP 2001-124621 5/2001
 WO WO9305503 A1 3/1993
 WO WO95/16259 A1 6/1995
 WO WO01/56328 A1 8/2001
 WO WO01/69968 A2 9/2001
 WO WO2006042540 A1 4/2006

OTHER PUBLICATIONS

F. Luo, J. Yang, C. Pavlovic, and A. Nehorai, "Adaptive null-forming scheme in digital hearing aids", IEEE Trans. Signal Process., vol. 50, pp. 1583-1590, 2002.*
 Gary W. Elko et al., "A simple adaptive first-order differential microphone," IEEE ASSP Workshop on New Paltz, NY, Oct. 15-18, 1995, XP010154658, 4 pages.
 Markus Buck, "Aspects of First-Order Differential Microphone Arrays in the Presence of Sensor Imperfections," European Transactions on Telecommunications, Wiley & Sons, Chichester, GB, vol. 13, No. 2, Mar. 2002, XP001123749, pp. 115-122.
 Sven Fischer et al., "Beamforming microphone arrays for speech acquisition in noisy environments," Speech Communication, Elsevier Science Publishers, Amsterdam, NL, vol. 20, No. 3, Dec. 1996, XP004016546, pp. 215-227.
 Restriction Requirement; Mailed Mar. 24, 2011 for corresponding U.S. Appl. No. 12/089,545.
 Non-Final Office Action; Mailed Jun. 22, 2011 for corresponding U.S. Appl. No. 12/089,545.
 Notice of Allowance; Mailed Sep. 21, 2011 for corresponding U.S. Appl. No. 12/089,545.
 Restriction Requirement; Mailed Jan. 16, 2006 for the corresponding U.S. Appl. No. 10/193,825.
 Non-Final Office Action; Mailed May 17, 2006 for the corresponding U.S. Appl. No. 10/193,825.
 Notice of Allowance; Mailed Oct. 16, 2006 for the corresponding U.S. Appl. No. 10/193,825.
 Communication Pursuant to Article 94(3) EPC; Mailed Mar. 30, 2012 for corresponding EP Application No. 07 752 770.3.
 Eargle, J.; "The Microphone Book"; 2nd Ed.; Focal Press; 2004; pp. 82-85.
 Communication Pursuant to Article 94(3) EPC; Mailed Jul. 5, 2012 for corresponding EP Application No. 07 752 770.3.

* cited by examiner

FIG. 1

100

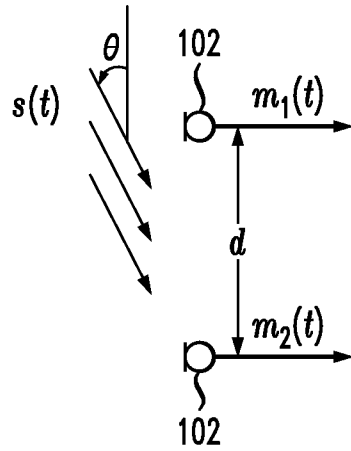


FIG. 2

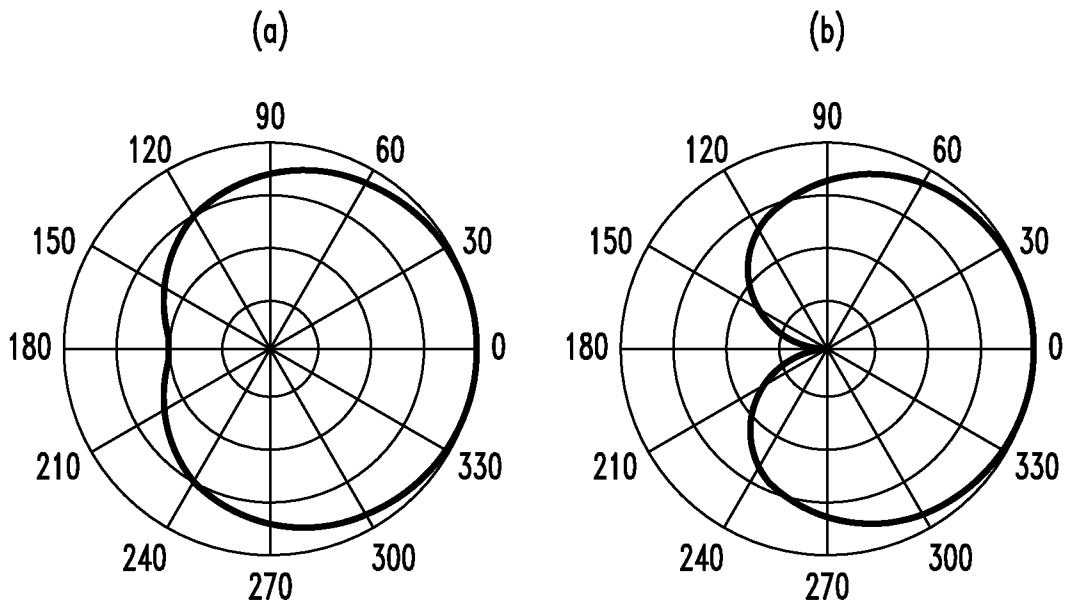


FIG. 3

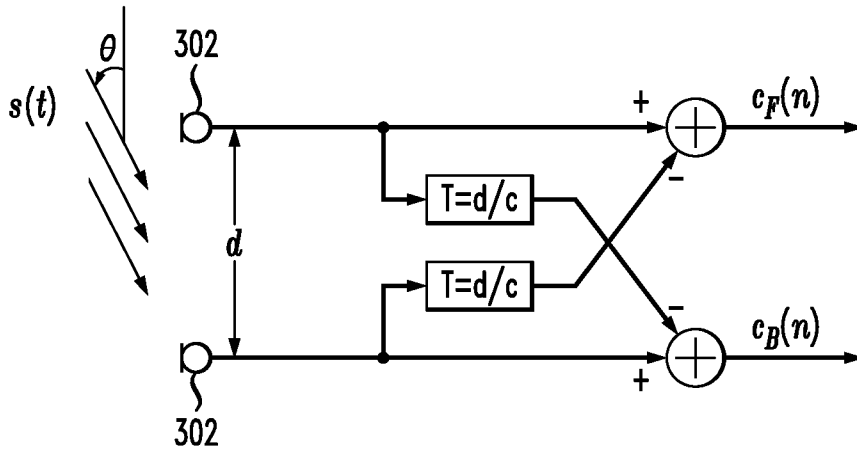


FIG. 4

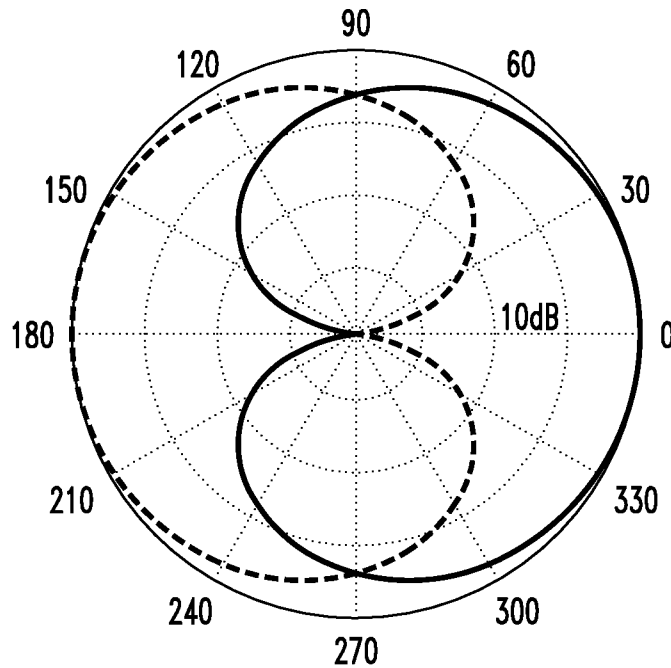


FIG. 5


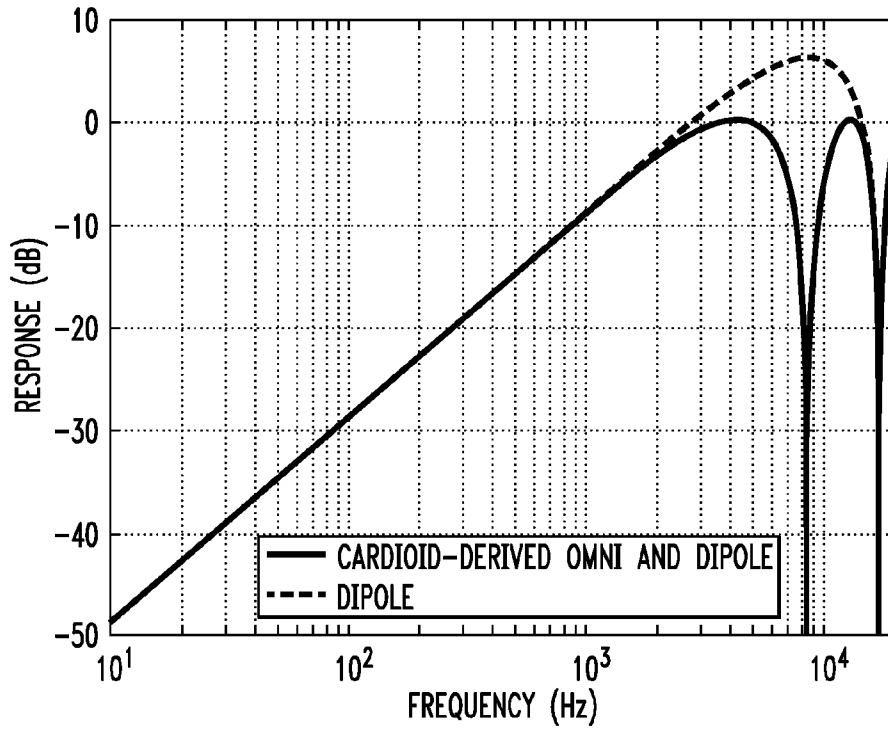


FIG. 6

600

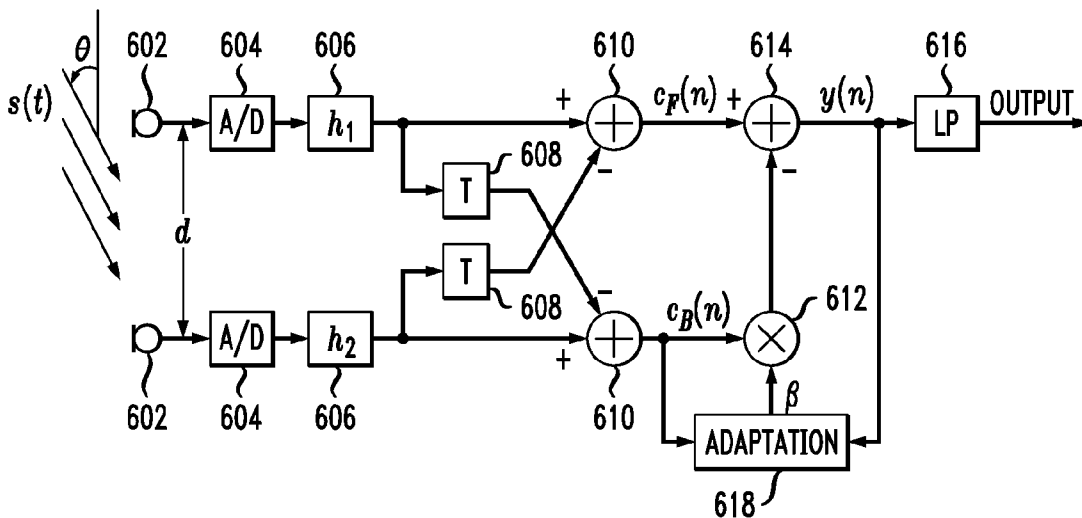

Explore Litigation Insights

Docket Alarm provides insights to develop a more informed litigation strategy and the peace of mind of knowing you're on top of things.

Real-Time Litigation Alerts



Keep your litigation team up-to-date with **real-time alerts** and advanced team management tools built for the enterprise, all while greatly reducing PACER spend.

Our comprehensive service means we can handle Federal, State, and Administrative courts across the country.

Advanced Docket Research



With over 230 million records, Docket Alarm's cloud-native docket research platform finds what other services can't. Coverage includes Federal, State, plus PTAB, TTAB, ITC and NLRB decisions, all in one place.

Identify arguments that have been successful in the past with full text, pinpoint searching. Link to case law cited within any court document via Fastcase.

Analytics At Your Fingertips



Learn what happened the last time a particular judge, opposing counsel or company faced cases similar to yours.

Advanced out-of-the-box PTAB and TTAB analytics are always at your fingertips.

API

Docket Alarm offers a powerful API (application programming interface) to developers that want to integrate case filings into their apps.

LAW FIRMS

Build custom dashboards for your attorneys and clients with live data direct from the court.

Automate many repetitive legal tasks like conflict checks, document management, and marketing.

FINANCIAL INSTITUTIONS

Litigation and bankruptcy checks for companies and debtors.

E-DISCOVERY AND LEGAL VENDORS

Sync your system to PACER to automate legal marketing.