



US005758644A

United States Patent [19]

Diab et al.

[11] **Patent Number:** **5,758,644**

[45] **Date of Patent:** **Jun. 2, 1998**

[54] **MANUAL AND AUTOMATIC PROBE CALIBRATION**

[75] Inventors: **Mohamed Kheir Diab**, Mission Viejo; **Massi E. Kiani**, Laguna Niguel; **Charles Robert Ragsdale**, Newport Beach; **James M. Lepper, Jr.**, Trabuco Canyon, all of Calif.

[73] Assignee: **Masimo Corporation**, Irvine, Calif.

[21] Appl. No.: **478,493**

[22] Filed: **Jun. 7, 1995**

[51] **Int. Cl.⁶** **A61B 5/00**

[52] **U.S. Cl.** **128/633; 128/664; 128/665; 356/41**

[58] **Field of Search** **128/633, 634, 128/664, 665; 356/39, 41; 315/151, 307, 310, 311; 250/552, 214 R**

[56] **References Cited**

U.S. PATENT DOCUMENTS

3,463,142	8/1969	Harte .	
3,647,299	3/1972	Lavallee .	
3,740,570	6/1973	Kaelin et al. .	
3,799,672	3/1974	Vurek .	
4,086,915	5/1978	Kofsky et al. .	
4,169,976	10/1979	Ciri .	
4,182,977	1/1980	Stricklin, Jr.	315/151
4,346,590	8/1982	Brown .	
4,407,290	10/1983	Wilber .	
4,449,821	5/1984	Lee .	
4,621,643	11/1986	New, Jr. et al. .	
4,653,498	3/1987	New, Jr. et al. .	
4,700,708	10/1987	New, Jr. et al. .	
4,770,179	9/1988	New, Jr. et al. .	
4,848,901	7/1989	Hood, Jr. .	
4,913,150	4/1990	Cheung et al. .	
4,942,877	7/1990	Sakai et al.	128/633
5,058,588	10/1991	Kaestle	128/633
5,113,862	5/1992	Mortazavi	128/633

5,140,228	8/1992	Biegel	315/310
5,267,562	12/1993	Ukawa et al.	128/633
5,287,853	2/1994	Vester et al.	128/633

FOREIGN PATENT DOCUMENTS

019478	11/1980	European Pat. Off. .	
5275746	10/1993	Japan .	
88/10462	12/1988	WIPO .	

OTHER PUBLICATIONS


Reynolds, K.J., et al. "Temperature Dependence of LED and its Theoretical Effect on Pulse Oximetry", *British Journal of Anaesthesia*, 1991, vol. 67, pp. 638-643.
de Kock, J.P. et al., "The Effect of Varying LED Intensity on Pulse Oximeter Accuracy", *Journal of Medical Engineering & Technology*, vol. 15, No. 3, May/June, 1991, pp. 111-116.

Primary Examiner—Jennifer Bahr
Assistant Examiner—Eric F. Winakur
Attorney, Agent, or Firm—Knobbe, Martens, Olsen & Bear

[57] **ABSTRACT**

The method and apparatus of the present invention provides a system wherein light-emitting diodes (LEDs) can be tuned within a given range by selecting their operating drive current in order to obtain a precise wavelength. The present invention further provides a manner in which to calibrate and utilize an LED probe, such that the shift in wavelength for a known change in drive current is a known quantity. In general, the principle of wavelength shift for current drive changes for LEDs is utilized in order to allow better calibration and added flexibility in the use of LED sensors, particularly in applications when the precise wavelength is needed in order to obtain accurate measurements. The present invention also provides a system in which it is not necessary to know precise wavelengths of LEDs where precise wavelengths were needed in the past. Finally, the present invention provides a method and apparatus for determining the operating wavelength of a light emitting element such as a light emitting diode.

26 Claims, 20 Drawing Sheets

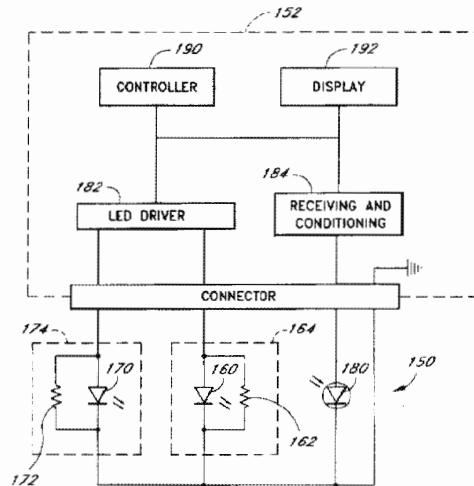

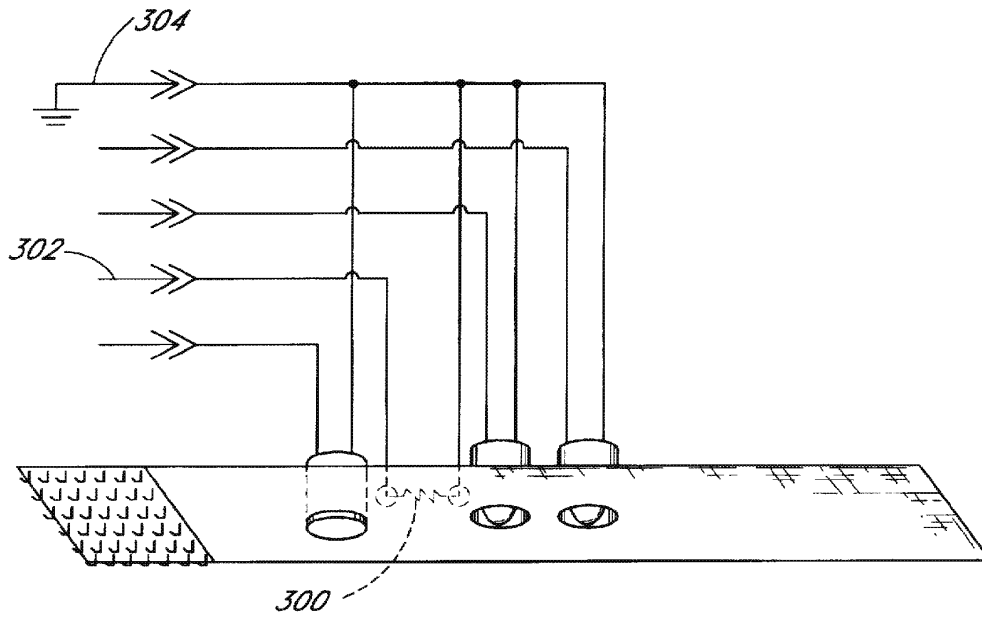


FIG. 1 (PRIOR ART)

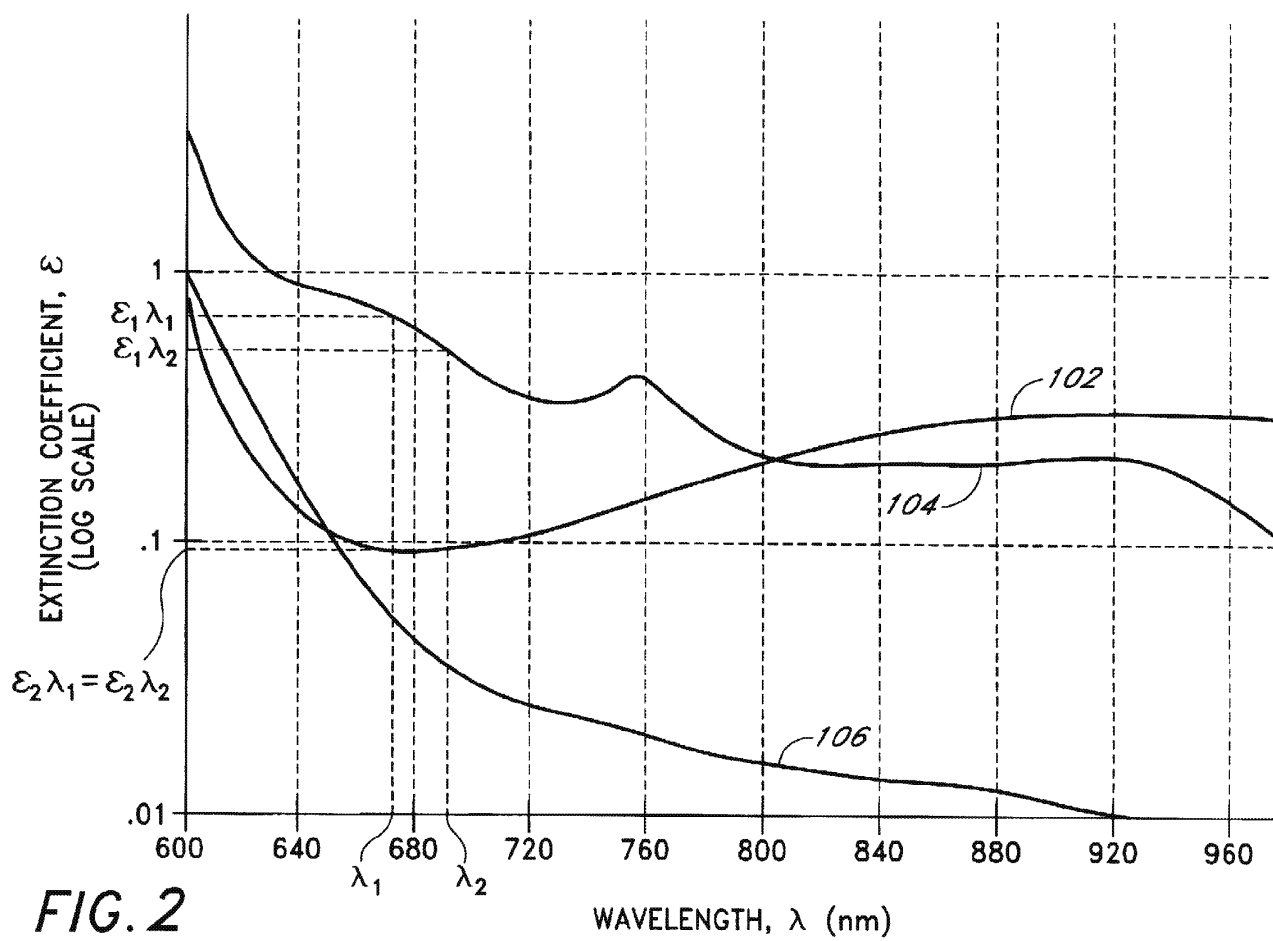


FIG. 2

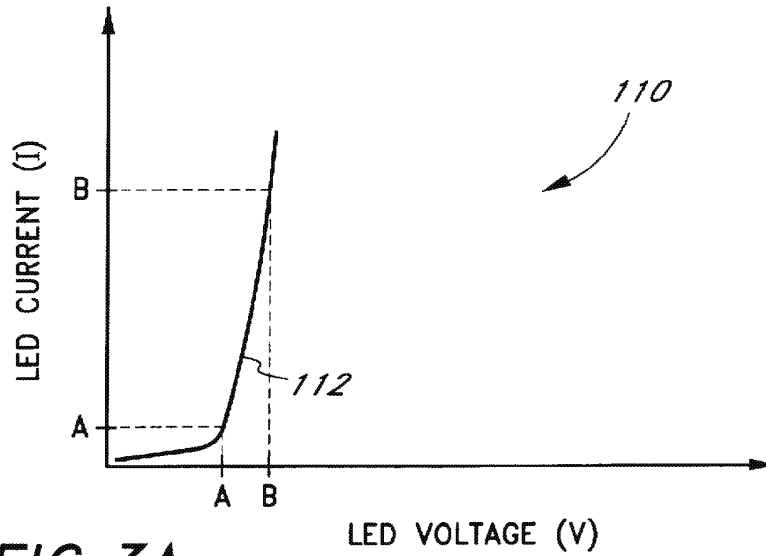


FIG. 3A


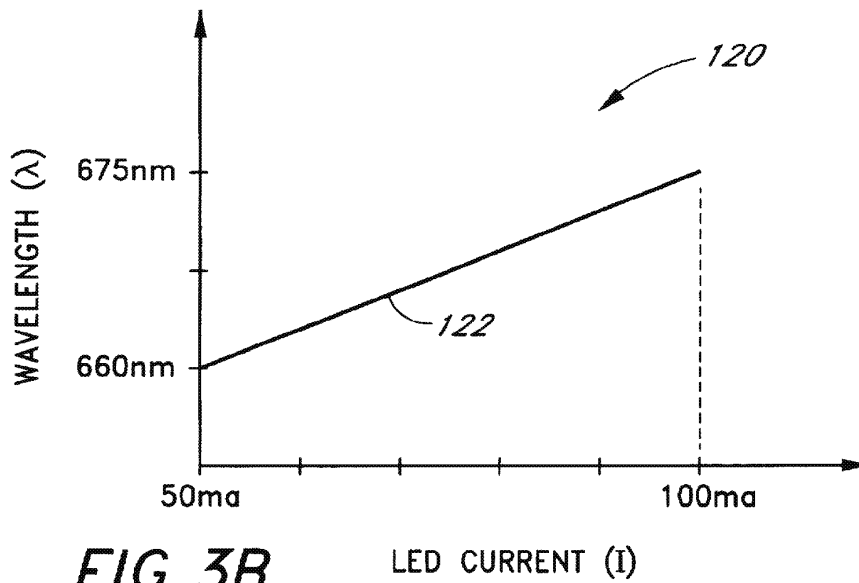


FIG. 3B

FIG. 4A

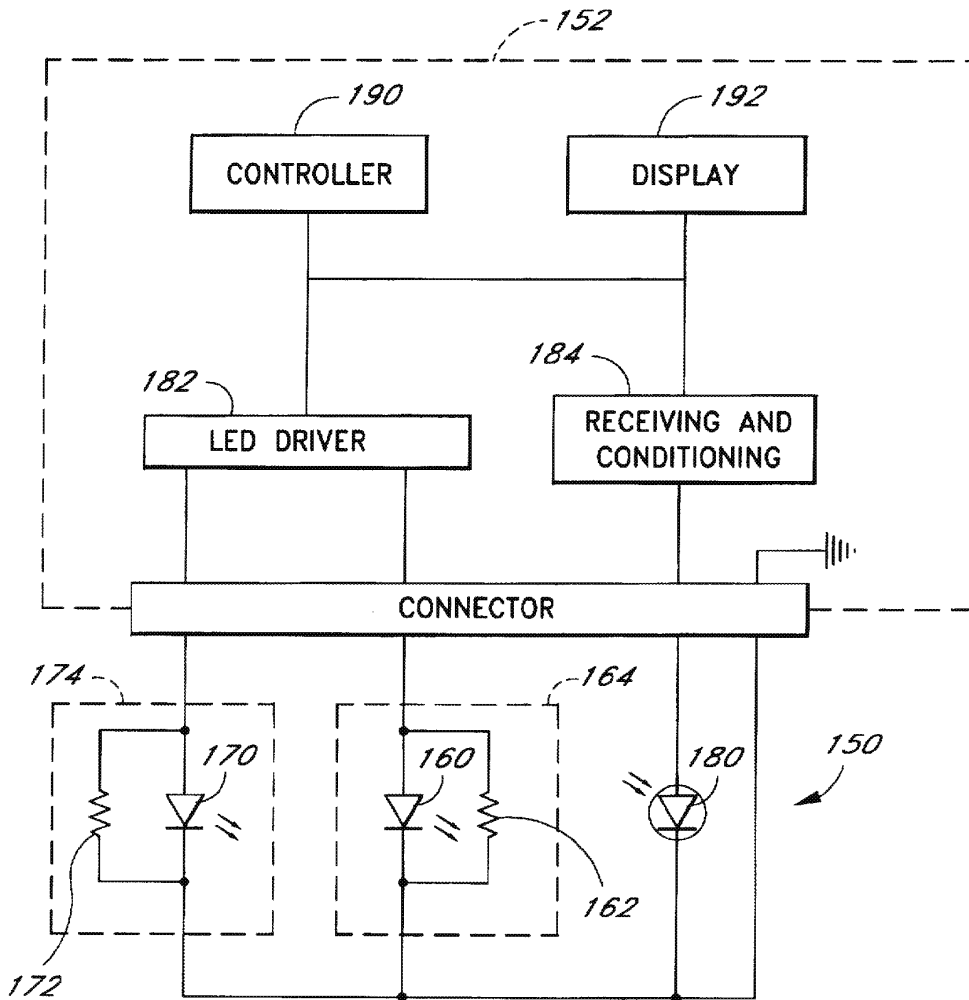

Explore Litigation Insights

Docket Alarm provides insights to develop a more informed litigation strategy and the peace of mind of knowing you're on top of things.

Real-Time Litigation Alerts



Keep your litigation team up-to-date with **real-time alerts** and advanced team management tools built for the enterprise, all while greatly reducing PACER spend.

Our comprehensive service means we can handle Federal, State, and Administrative courts across the country.

Advanced Docket Research



With over 230 million records, Docket Alarm's cloud-native docket research platform finds what other services can't. Coverage includes Federal, State, plus PTAB, TTAB, ITC and NLRB decisions, all in one place.

Identify arguments that have been successful in the past with full text, pinpoint searching. Link to case law cited within any court document via Fastcase.

Analytics At Your Fingertips



Learn what happened the last time a particular judge, opposing counsel or company faced cases similar to yours.

Advanced out-of-the-box PTAB and TTAB analytics are always at your fingertips.

API

Docket Alarm offers a powerful API (application programming interface) to developers that want to integrate case filings into their apps.

LAW FIRMS

Build custom dashboards for your attorneys and clients with live data direct from the court.

Automate many repetitive legal tasks like conflict checks, document management, and marketing.

FINANCIAL INSTITUTIONS

Litigation and bankruptcy checks for companies and debtors.

E-DISCOVERY AND LEGAL VENDORS

Sync your system to PACER to automate legal marketing.